

04/20/00

3639 U.S. PTO

UTILITY  
PATENT APPLICATION  
TRANSMITTAL

(Only for new nonprovisional applications under 37 CFR 1.53(b))


Attorney Docket No.	0163-0758-0X
First Inventor or Application Identifier	Ryuichiro KURANE
Title	METHOD FOR DETERMINING A CONCENTRATION OF TARGET NUCLEIC ACID MOLECULES, NUCLEIC ACID PROBES FOR THE METHOD, AND METHOD FOR ANALYZING DATA OBTAINED BY THE METHOD

3642 U.S. PTO

09/556127

04/20/00

<b>APPLICATION ELEMENTS</b> See MPEP chapter 600 concerning utility patent application contents	<b>ADDRESS TO:</b> Assistant Commissioner for Patents Box Patent Application Washington, DC 20231
<p>1. <input checked="" type="checkbox"/> Fee Transmittal Form (e.g. PTO/SB/17) (Submit an original and a duplicate for fee processing)</p> <p>2. <input checked="" type="checkbox"/> Specification Total Pages <b>123</b></p> <p>3. <input checked="" type="checkbox"/> Drawing(s) (35 U.S.C. 113) Total Sheets <b>14</b></p> <p>4. <input type="checkbox"/> Oath or Declaration Total Pages <input type="text"/></p> <p>a. <input type="checkbox"/> Newly executed (original or copy)</p> <p>b. <input type="checkbox"/> Copy from a prior application (37 C.F.R. §1.63(d)) (for continuation/divisional with box 15 completed)</p> <p>i. <input type="checkbox"/> <b>DELETION OF INVENTOR(S)</b> Signed statement attached deleting inventor(s) named in the prior application, see 37 C.F.R. §1.63(d)(2) and 1.33(b).</p> <p><input type="checkbox"/> Incorporation By Reference (usable if box 4B is checked) The entire disclosure of the prior application, from which a copy of the oath or declaration is supplied under Box 4B, is considered to be part of the disclosure of the accompanying application and is hereby incorporated by reference therein.</p>	<b>ACCOMPANYING APPLICATION PARTS</b> <p>6. <input type="checkbox"/> Assignment Papers (cover sheet &amp; document(s))</p> <p>7. <input type="checkbox"/> 37 C.F.R. §3.73(b) Statement (when there is an assignee) <input type="checkbox"/> Power of Attorney</p> <p>8. <input type="checkbox"/> English Translation Document (if applicable)</p> <p>9. <input checked="" type="checkbox"/> Information Disclosure Statement (IDS)/PTO-1449 <input checked="" type="checkbox"/> Copies of IDS Citations</p> <p>10. <input type="checkbox"/> Preliminary Amendment</p> <p>11. <input checked="" type="checkbox"/> White Advance Serial No. Postcard</p> <p>12. <input type="checkbox"/> Small Entity Statement(s) <input type="checkbox"/> Statement filed in prior application. Status still proper and desired.</p> <p>13. <input type="checkbox"/> Certified Copy of Priority Document(s) (if foreign priority is claimed)</p> <p>14. <input checked="" type="checkbox"/> Other: <b>REQUEST FOR PRIORITY; LIST OF INVENTORS NAMES AND ADDRESSES</b></p>
<p>15. If a CONTINUING APPLICATION, check appropriate box, and supply the requisite information below:</p> <p><input type="checkbox"/> Continuation <input type="checkbox"/> Divisional <input type="checkbox"/> Continuation-in-part (CIP) of prior application no.: Prior application information: Examiner: Group Art Unit:</p>	
<p>16. Amend the specification by inserting before the first line the sentence:</p> <p><input type="checkbox"/> This application is a <input type="checkbox"/> Continuation <input type="checkbox"/> Division <input type="checkbox"/> Continuation-in-part (CIP) of application Serial No. Filed on</p> <p><input type="checkbox"/> This application claims priority of provisional application Serial No. Filed</p>	
<p><b>17. CORRESPONDENCE ADDRESS</b></p> <p>OBLON, SPIVAK, MCCLELLAND, MAIER &amp; NEUSTADT, P.C. FOURTH FLOOR 1755 JEFFERSON DAVIS HIGHWAY ARLINGTON, VIRGINIA 22202 (703) 413-3000 FACSIMILE: (703) 413-2220</p>	

Name:	Norman F. Oblon	Registration No.:	24,618
Signature:		Date:	04/20/00
Name:	Daniel J. Pereira, Ph.D.	Registration No.:	45,518

METHOD FOR DETERMINING A CONCENTRATION OF TARGET  
NUCLEIC ACID MOLECULES, NUCLEIC ACID PROBES FOR THE METHOD,  
AND METHOD FOR ANALYZING DATA OBTAINED BY THE METHOD

5

BACKGROUND OF THE INVENTION

a) Field of the Invention

10

15

20

25

This invention relates to a method for determining a concentration of a target nucleic acid, a nucleic acid probe for the process, and a method for analyzing data obtained by the method. Specifically, the present invention is concerned with various methods for determining concentrations of diverse nucleic acids on the basis of a principle that fluorescence emission from of a fluorescent dye decreases when a nucleic acid probe labeled with the fluorescent dye is hybridized to a target nucleic acid, that is, by measuring decreases in fluorescence emissions from fluorescent dyes after hybridization of nucleic acid probes labeled with the fluorescent dyes to target nucleic acids relative to fluorescence emissions from the fluorescent dyes before the hybridization, nucleic acid probes and devices useful for the practice of the methods, methods for analyzing data obtained by PCR which is one of the determination methods, systems provided with means for practicing the analysis methods, and computer-readable recording media with individual procedures of the analysis methods stored therein as programs.

b) Description of the Related Art

00556127.042000  
000240/22195560

A variety of methods are conventionally known to determine a concentration of a nucleic acid by using a nucleic acid probe labeled with a fluorescent dye. These methods include:

5 (1) Dot blotting assay

After a target nucleic acid and a nucleic acid probe labeled with a fluorescent dye are hybridized on a membrane, unreacted nucleic probe is washed off. The intensity of fluorescence only from fluorescent dye molecules, by which the nucleic acid probe hybridized with the target nucleic acid is labeled, is measured.

(2) Method making use of an intercalator: Glazer et al., Nature, 359, 959, 1992

A certain specific fluorescent dye called "intercalator" emits strong fluorescence upon its insertion into a double strand of a nucleic acid. This method measures an increase in fluorescence from the fluorescent dye. Examples of the fluorescent dye can include ethidium bromide [Jikken Igaku (Laboratory Medicine), 15(7), 46-51, Yodosha (1997)] and SYBR R Green I (LightCycler™ System, April 5, 1999; pamphlet distributed by Roche Diagnostics, Mannheim, Germany).

(3) Method making use of FRET (fluorescence energy transfer): Mergny et al., Nucleic Acid Res., 22, 920-928, 1994

This method comprises hybridizing two nucleic acid probes to a target nucleic acid. These two nucleic acid probes are

labeled by different fluorescent dyes, respectively. The fluorescent dye of one of the two probes can transfer energy to the fluorescent dye of the other probe such that the latter fluorescent dye is caused to emit fluorescence. These two probes are designed such that they hybridize with their fluorescent dyes being located opposite each other and apart from each other by 1 to 9 bases. When these two nucleic acid probes hybridize to the target nucleic acid, emission of fluorescence from the latter fluorescent dye takes place. The intensity of this fluorescence emission is proportional to the number of replications of the target nucleic acid.

(4) Molecular beacon method: Tyagi et al., Nature Biotech., 14, 303-308, 1996

A nucleic acid probe for use in this method is labeled at an end thereof with a reporter dye and at an opposite end thereof with a quencher dye. As both end portions of the probe are complementary with each other in their base sequences, the overall base sequence of the probe is designed to form a hairpin stem. Owing to this structure, emission from the reporter dye is suppressed by the quencher dye under Forster resonant energy in a state suspended in a liquid. When the probe hybridizes to a target nucleic acid, the hairpin stem structure is broken. This leads to an increase in the distance between the reporter pigment and the quencher pigment, so that the transfer of Forster resonant energy no longer takes place. This allows the



reporter dye to make emission.

(5) Davis's method: Davis et al., Nucleic Acids Res., 24,  
702-706, 1996

This method uses DNA constructs containing one or two  
fluorescein molecules in flow cytometry. The fluorescein  
molecules were attached to the 3' end of a DNA probe through an  
18-atom spacer arm that resulted in a 10-fold increase in  
fluorescence intensity compared to the DNA probe to which  
fluorescein was directly attached to the 3' end of the probe.

Applied to various determination methods for nucleic  
acids, fluorescent in situ hybridization assays, PCR, ligase  
chain reactions, strand displacement assays, competitive  
hybridization and the like, significant developments have been  
made on these methods.

Although these methods are now widely used, they include  
a disadvantageous step that, subsequent to hybridization  
reaction between a nucleic acid probe labeled with a fluorescent  
dye and a target nucleic acid, an unhybridized portion of the  
nucleic acid probe has to be washed out of the reaction system.  
Obviation of this step can apparently bring about shorter  
determination time, simplified determination, and accurate  
determination. There is, accordingly, a long-standing desire  
for the development of a nucleic acid determination method which  
does not include such a step.

SUMMARY OF THE INVENTION

With the foregoing in view, the present invention has as an object thereof the provision of a method for determining a concentration of a target nucleic acid by using a nucleic acid probe labeled with a fluorescent dye, which makes it possible to determine the concentration of the target nucleic acid in a shorter time, more easily and more accurately.

The present invention also has as other objects the provision of nucleic acid probes and devices useful for the practice of the methods, methods for analyzing data obtained by PCR which is one of the determination methods, systems provided with means for practicing the analysis methods, and computer-readable recording media with individual procedures of the analysis methods stored therein as programs.

To achieve the above-described objects, the present inventors have proceeded with an investigation on methods for determining a concentration of a nucleic acid by using a nucleic acid probe. As a result, it was found that emission of fluorescence from a fluorescent dye decreases (quenching phenomenon of fluorescence) when a nucleic acid probe labeled with the fluorescent dye hybridizes to a target nucleic acid. It was also found that this decrease is significant with certain specific dyes. It was also found that the extent of this decrease varies depending on bases in a probe portion, to which the fluorescent dye is conjugated, or on the sequence of the

bases. The present invention has been completed base on these findings.

Therefore, the present invention provides the following methods, probes, kits, systems, recording medium, device and assay:

1) A method for determining a concentration of a target nucleic acid by using a nucleic acid probe labeled with a fluorescent dye, which comprises:

providing, as the probe, a nucleic acid probe capable of reducing fluorescence emission from the fluorescent dye when hybridized with the target nucleic acid;

hybridizing the probe to the target nucleic acid; and

measuring a decrease in fluorescence emission from the fluorescent dye after the hybridization relative to fluorescence emission from the fluorescent dye before the hybridization.

2) A nucleic acid probe for determining a concentration of a target nucleic acid, said probe being labeled with a fluorescent dye, wherein:

the probe is labeled at an end portion thereof with the fluorescent dye, and

the probe has a base sequence designed such that, when the probe is hybridized with the target nucleic acid, at least one G (guanine) base exists in a base sequence of the target nucleic acid at a position 1 to 3 bases apart from an end base

portion where the probe and the target nucleic acid are hybridized with each other,

whereby the fluorescent dye is reduced in fluorescence emission when the probe is hybridized with the target nucleic acid; and

a method for determining a concentration of a target nucleic acid, which comprises hybridizing the above-described nucleic acid probe to the target nucleic acid and measuring a decrease in fluorescence emission from the fluorescent dye after the hybridization relative to fluorescence emission from the fluorescent dye before the hybridization.

3) A method for analyzing or determining polymorphism or mutation of a target nucleic acid or gene, which comprises:

hybridizing the above-described nucleic acid probe to the target nucleic acid or gene, and measuring a change in fluorescence.

4) A kit for analyzing or determining polymorphism or mutation of a target nucleic acid or gene, comprising the above-described nucleic acid probe.

5) A method for analyzing data obtained by the analysis or determination method described above under 3), which comprises the following step:

correcting a fluorescence intensity of a reaction system, in which the target nucleic acid or gene has been hybridized with the nucleic acid probe labeled with the fluorescent dye,

000240 22795500

in accordance with a fluorescence intensity of the reaction system before the hybridization.

6) A system for analyzing or determining polymorphism or mutation of a target nucleic acid or gene, comprising means for practicing the data analysis or determination method described above under 5).

7) A computer-readable, recording medium comprising a program recorded therein for making a computer perform the correction step described above under 5).

8) A method for determining a concentration of a target nucleic acid, which comprises using a probe with the nucleic acid probe described above under 1) or 2) bound on a surface of a solid support; and

a device for determining a concentration of the target nucleic acid, which is useful in practicing the above method.

9) A fluorescent in situ hybridization assay making use of the nucleic acid determination method described above under 1), 2) or 8).

10) A method for analyzing data obtained by the nucleic acid determination method described above under 1), 2) or 9).

11) A PCR method making use of the nucleic acid determination method described above under 1) or 2).

12) A method for analyzing data obtained by the PCR method described above under 11).

13) A method for analyzing a melting curve of a nucleic acid

000240 2219550

by using the PCR method described above under 11).

14) An analysis method making combined use of the methods described above under 12) and 13), respectively.

5 15) A PCR determination and/or analysis system provided with means for performing an analysis in accordance with the analysis method described above under 11), 12), 13) or 14).

10 16) A computer-readable recording medium with procedures, through which an analysis is performed by the analysis method described above under 11), 12), 13) or 14), recorded as a program.

17) A method for quantitating a target nucleic acid, which comprises making use of the data analysis method described above under 12) or 14).

15 18) A method for determining a concentration of a target nucleic acid, which comprises using the PCR determination and/or analysis system described above under 15).

19) A method for determining a concentration of a target nucleic acid, which comprises using the recording medium described above under 16).

20 Numerous advantageous effects have been brought about by the present invention as will be set out below.

1) Since use of the nucleic acid determination method, probe or device according to the present invention does not require an operation such as that needed to remove unreacted nucleic acid probe from a determination system, the concentration of

25

0556127.042000

a target nucleic acid can be determined in a short time and with ease. When applied to a co-cultivation system of microorganisms or a symbiotic cultivation system of microorganisms, the viable count of a particular microorganism strain in the system can be specifically measured in a short time. Further, the present invention has also provided a simple method for analyzing or determining polymorphism, such as SNP (single nucleotide polymorphism), or mutation of a target nucleic acid or gene.

2) Further, the quantitative PCR method according to the present invention has the following advantageous effects:

- a. As the quantitative PCR method does not involve addition of any factor which may act in an inhibitive manner on amplification of a target nucleic acid by Taq DNA polymerase, quantitative PCR can be conducted under similar conditions as conventionally-known usual PCR having specificity.
- b. The specificity of PCR can be maintained high, so that amplification of primer dimer is retarded. Compared with conventionally-known quantitative PCR, the quantitation limit can be lowered on the order of about one digit.
- c. It is no longer required to provide a complex nucleic acid probe. It is, therefore, possible to save time and cost which would otherwise be required for such

a complex nucleic acid probe.

d. A target nucleic acid can be effectively amplified, so that the amplification step can be monitored in real time.

5 3) Upon analysis of data obtained by the real-time  
quantitative PCR, the data analysis method according to the  
present invention can be used to prepare a working line for the  
determination of the number of copies of a nucleic acid in a  
nucleic acid sample of unknown nucleic acid copy number. This  
10 working line has a correlation coefficient which is far higher  
than those available by conventional methods. Use of the data  
analysis method according to the present invention, therefore,  
makes it possible to accurately determine the number of copies  
of nucleic acid.

4) A working line the correlation efficient of which is high can be automatically prepared by the use of the data analysis software relating to the analysis method of data obtained by real-time quantitative PCR, the computer-readable recording medium with the procedures of the analysis method recorded as a program therein, or the determination or analysis system for the real-time quantitative PCR. The data analysis software, computer-readable recording medium, and the determination or analysis system all pertain to the present invention.

5) Further, use of the novel method according to the present  
invention for the analysis of the melting curve of a nucleic

[illegible]



acid makes it possible to determine the  $T_m$  value of the nucleic acid with high accuracy. Moreover, use of the data analysis software for the method, the computer-readable recording medium with the procedures of the analysis method recorded as a program therein, or the determination or analysis system for the real-time quantitative PCR makes it possible to obtain an accurate  $T_m$  value.

#### BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a diagram showing measurement data of fluorescence intensity when the sequence of bases in 16S rRNA of *Escherichia coli*, said bases ranging from the 335<sup>th</sup> base to the 358<sup>th</sup> base as counted from the 5' end, was determined using a nucleic acid probe obtained in Example 1;

FIG. 2 diagrammatically illustrates effects of heat treatment of 16S rRNA on hybridization of a 35-nucleotides-chained 2-O-Me probe to a target nucleic acid, in which:

Dashed curve: Heated 16S rRNA was added to a solution of the probe, and

Solid curve: Non-heated 16S rRNA was added to a solution of the probe;

FIG. 3 diagrammatically shows effects of methylation of 2'-OH of ribose in the 5' terminal residue of the probe, the number of nucleotide-chain of the probe and the helper probes on the hybridization of the probes to the target 16S rRNA;

FIG. 4 shows a working curve of rRNA assay by an invention method;

FIG. 5 diagrammatically shows analysis results of time-dependent rRNA of the strains, KYM-7 and KYM-8, in co-cultivation by an in situ hybridization assay method with the invention technique;

FIG. 6 is a schematic illustration of a DNA chip according to the present invention;

FIG. 7 diagrammatically illustrates a relationship between cycles and a decrease in fluorescence emission from a fluorescent dye in a real-time quantitative PCR method making use of primers 1 and 2 labeled with BODIPY FL, in which signs ① to ⑧ have the following meanings:

① Number of copies of *E. coli* genome DNA: 0;

primer: primer 1 + primer 2.

② Number of copies of *E. coli* genome DNA:  $2.4 \times 10^6$ ;

primer: primer 1 + primer 2.

③ Number of copies of *E. coli* genome DNA:  $2.4 \times 10^5$ ;

primer: primer 1 + primer 2.

④ Number of copies of *E. coli* genome DNA:  $2.4 \times 10^4$ ;

primer: primer 1 + primer 2.

⑤ Number of copies of *E. coli* genome DNA:  $2.4 \times 10^3$ ;

primer: primer 1.

⑥ Number of copies of *E. coli* genome DNA:  $2.4 \times 10^2$ ;

primer: primer 1.

⑦ Number of copies of *E. coli* genome DNA:  $2.4 \times 10^4$ ;  
primer: primer 1.

⑧ Number of copies of *E. coli* genome DNA:  $2.4 \times 10^0$ ;  
primer: primer 1.

FIG. 8 diagrammatically shows a relationship between cycles and the logarithm of a decrease in fluorescence emission from a fluorescent dye in the real-time quantitative PCR making use of primers 1 and 2 labeled with BODIPY FL, in which signs ① to ⑧ have the same meanings as defined above in connection with FIG. 7;

FIG. 9 is a diagram showing a working line for 16S rDNA of *Escherichia coli*, which was prepared using the real-time quantitative PCR according to the present invention;

FIG. 10 (upper diagram) depicts decreases (%) in  
15 fluorescence intensity in real-time quantitative PCR according  
to the present invention in which a single probe of the present  
invention was used as opposed to two probes required for a  
conventional real-time quantitative PCR method using FRET;

FIG. 10 (lower diagram) shows a working line for 16S rDNA of *Escherichia coli*, and the working line depicts a relationship between the number of copies of the 16S rDNA and starting cycles (threshold cycle numbers) in each copy of the nucleic acid at which the decrease in fluorescence emission was capable of being significantly observed in the upper diagram;

25 FIG. 11 depicts fluorescence decrease curves obtained by

real-time quantitative PCR according to the present invention, which used a primer labeled with BODIPY FL, without performing correction processing according to the present invention, in which:

- 5           ■ Target nucleic acid: 10 copies; Temperature of the reaction system upon measurement of fluorescence intensity: 72°C.
- 10           ● Target nucleic acid: 100 copies; Temperature of the reaction system upon measurement of fluorescence intensity: 72°C.
- ▲ Target nucleic acid: 1,000 copies; Temperature of the reaction system upon measurement of fluorescence intensity: 72°C.
- 15           ◆ Target nucleic acid: 10,000 copies; Temperature of the reaction system upon measurement of fluorescence intensity: 72°C.
- Target nucleic acid: 10 copies; Temperature of the reaction system upon measurement of fluorescence intensity: 95°C.
- 20           ○ Target nucleic acid: 100 copies; Temperature of the reaction system upon measurement of fluorescence intensity: 95°C.
- △ Target nucleic acid: 1,000 copies; Temperature of the reaction system upon measurement of fluorescence intensity: 95°C.
- 25

◇ Target nucleic acid: 10,000 copies; Temperature of the reaction system upon measurement of fluorescence intensity: 95°C.

FIG. 12 shows fluorescence decrease curves obtained by the real-time quantitative PCR according to the present invention as in FIG. 11 except that on each of the curves, each decrease (%) in fluorescence emission was corrected assuming that the corresponding value in the 10<sup>th</sup> cycle was 1, in which:

- Target nucleic acid: 10 copies; Temperature upon measurement of fluorescence intensity: 72°C.
- Target nucleic acid: 100 copies; Temperature upon measurement of fluorescence intensity: 72°C.
- ▲ Target nucleic acid: 1,000 copies; Temperature upon measurement of fluorescence intensity: 72°C.
- ◆ Target nucleic acid: 10,000 copies; Temperature upon measurement of fluorescence intensity: 72°C.

FIG. 13 shows curves obtained by calculating, with respect to the individual plotted values on the respective curves in FIG. 12, the rates of decreases (the rates of changes) in fluorescence intensity in accordance with the formula (9) and then plotting the thus-calculated, in which:

- Target nucleic acid: 10 copies.
- Target nucleic acid: 100 copies.
- ▲ Target nucleic acid: 1,000 copies.
- ◆ Target nucleic acid: 10,000 copies.

FIG. 14 shows a working line for human genome DNAs as obtained from the data in FIG. 13, in which:

y: Number of copies of human  $\beta$ -globin gene,

x: cycles (Ct), and

$R^2$ : correlation coefficient.

FIG. 15 depicts curves obtained by subjecting the measurement values in the individual cycles in FIG. 11 to correction processing in accordance with the formula (1) and then plotting the corrected values relative to their corresponding cycles, in which:

■ Target nucleic acid: 10 copies.

● Target nucleic acid: 100 copies.

▲ Target nucleic acid: 1,000 copies.

◆ Target nucleic acid: 10,000 copies.

FIG. 16 illustrates curves obtained by plotting values, which have been obtained by processing the processed values of the individual cycles in FIG. 15 in accordance with the formula (3), against their corresponding cycles, in which

■ Target nucleic acid: 10 copies.

● Target nucleic acid: 100 copies.

▲ Target nucleic acid: 1,000 copies.

◆ Target nucleic acid: 10,000 copies.

FIG. 17 shows curves obtained by subjecting the corrected values in the individual cycles in FIG. 16 to correction processing in accordance with the formula (6) and then plotting

the corrected values relative to their corresponding cycles,  
in which:

- Target nucleic acid: 10 copies.
- Target nucleic acid: 100 copies.
- ▲ Target nucleic acid: 1,000 copies.
- ◆ Target nucleic acid: 10,000 copies.

FIG. 18 shows working lines drawn corresponding to 0.1,  
0.3, 0.5, 0.7, 0.9 and 1.2 chosen at will as candidates for  
threshold cycle numbers from the respective values of log  
(changes in fluorescence, %) in FIG. 16, in which the individual  
working lines have the following correlation coefficients:

- ▲  $\log (\text{change in fluorescence, \%}) = 0.1;$   
correlation coefficient: 0.998
- $\log (\text{change in fluorescence, \%}) = 0.3;$   
correlation coefficient: 0.999
- $\log (\text{change in fluorescence, \%}) = 0.5;$   
correlation coefficient: 0.9993
- △  $\log (\text{change in fluorescence, \%}) = 0.7$   
correlation coefficient: 0.9985
- $\log (\text{change in fluorescence, \%}) = 0.9$   
correlation coefficient: 0.9989
- $\log (\text{change in fluorescence, \%}) = 1.2$   
correlation coefficient: 0.9988

FIG. 19 depicts fluorescence decrease curves when  
real-time quantitative PCR according to the present invention

was conducted on human genome DNA of 1 copy and 10 copies by using the primer labeled with BODIPY FL and the correction processing of the formula (1) was applied, in which:

- 1: target nucleic acid = 0 copy,
- 2: target nucleic acid = 1 copy, and
- 3: target nucleic acid = 10 copies;

FIG. 20 illustrates melting curves of nucleic acids when a melting curve analysis was conducted with respect to the PCR amplification products shown in FIG. 19, in which:

- 1: target nucleic acid = 0 copy,
- 2: target nucleic acid = 1 copy, and
- 3: target nucleic acid = 10 copies; and

FIG. 21 illustrates curves obtained by differentiating the curves of FIG. 20 and showing  $T_m$  values as valleys, in which:

- 2: target nucleic acid: 1 copy, and
- 3: target nucleic acid: 10 copies.

#### DETAILED DESCRIPTION OF THE INVENTION

##### AND PREFERRED EMBODIMENTS

The present invention will next be described in further detail based on certain preferred embodiments.

The terms as used herein - such as DNAs, RNAs, cDNAs, mRNAs, rRNAs, XTPs, dXTPs, NTPs, dNTPs, nucleic acid probes, helper nucleic acid probes (or nucleic acid helper probes, or simply helper probes), to hybridize, hybridization, intercalators,



primers, annealing, extending reactions, thermal denaturing reactions, nucleic acid melting curves, PCR, RT-PCR, RNA-primed PCR, stretch PCR, reverse PCR, PCR using mixed primers, PCR using PNA, hybridization assays, fluorescent in situ

5 hybridization assays, polymerase chain assays (PCR methods),  
ligase chain reactions, strand displacement assays,  
competitive hybridization, DNA chips, nucleic acid detecting  
(gene-detecting) devices, SNP (single nucleotide  
polymorphism), and co-cultivation systems of plural  
10 microorganisms - have the same meanings as the corresponding  
terms generally employed these days in molecular biology,  
genetic engineering, bioengineering and the like.

A first feature of the present invention resides in that,  
in a method for determining a concentration of a target nucleic  
15 acid by using a nucleic acid probe labeled with a fluorescent  
dye, a decrease in fluorescent emission from the fluorescent  
dye, said decrease taking place upon hybridization of the  
nucleic acid probe to the target nucleic acid, in other words,  
a decrease in fluorescent emission from the fluorescent dye  
20 after the hybridization relative to fluorescent emission from  
the fluorescent dye before the hybridization is measured.

The expression "measurement of a target nucleic acid" as  
used herein means quantitation or quantitative detection of the  
target nucleic acid or mere detection of the target nucleic  
25 acid.

000240 2275560

The expression "method for determining a concentration of a target nucleic acid by using a nucleic acid probe labeled with a fluorescent dye" means a hybridization assay, fluorescent in situ hybridization assay, polymerase chain assay (PCR method), ligase chain reaction, strand displacement assay, competitive hybridization or the like. According to these methods, subsequent to addition of a nucleic acid probe labeled with a fluorescent dye, the fluorescent dye in the unreacted nucleic acid probe not hybridized with a target nucleic acid is removed from the determination system by washing or the like. The fluorescent dye, with which the nucleic acid probe hybridized with the target nucleic acid is labeled, is caused to emit fluorescence from the probe directly or by applying an indirect measure to the probe (for example, causing an enzyme to act), and the intensity of the fluorescence is measured. The present invention is characterized in that a concentration of a target nucleic acid is determined without needing such a complex operation.

The term "target nucleic acid" as used herein means a nucleic acid the quantitation or qualitative detection or mere detection of which is intended, irrespective whether it is in a purified form or not and further irrespective of its concentration. Various other nucleic acids may also exist together with the target nucleic acid. For example, the target nucleic acid may be a specific nucleic acid in a co-cultivation

system microorganisms (a mixed system of RNAs or gene DNAs of plural microorganisms) or a symbiotic cultivation system of microorganisms (a mixed system of RNAs or gene DNAs of plural animals, plants and/or microorganisms), the quantitation or qualitative detection or mere detection of which is intended. Purification of the specific nucleic acid, if needed, can be conducted by a method known per se in the art. For example, purification can be effected using a purification kit or the like available on the market. Specific examples of the above-described nucleic acid can include DNAs, RNAs, PNAs, 2-O-MeRNAs, deoxyribooligonucleotides, and riboxy-origonucleotides.

In the present invention, fluorescent dyes commonly employed for the determination or detection of nucleic acids by labeling nucleic acid probes may be conveniently used. It is, however, preferred to use fluorescent dyes the fluorescence emission from each of which decreases when a nucleic acid probe labeled with the fluorescent dye is hybridized to a target nucleic acid. Illustrative of such fluorescent dyes are fluorescein and derivatives thereof [for example, fluorescein isothiocyanate (FITC) and its derivatives]; Alexa 488, Alexa 532, cy3, cy5, EDANS (5-(2'-aminoethyl)amino-1-naphthalene sulfonic acid); rhodamine 6G (R6G) and its derivatives [for example, tetramethylrhodamine (TMR), tetramethylrhodamine isothiocyanate (TMRITC), x-rhodamine, Texas red, "BODIPY FL"

000240" 22795560



oligodeoxynucleotide is used primarily for the determination of RNA. Upon determination of RNA by the probe, it is preferred to subject an RNA solution as a sample to heat treatment at 80 to 100°C, preferably 90 to 100°C, most preferably 93 to 97°C for 1 to 15 minutes, preferably 2 to 10 minutes, most preferably 3 to 7 minutes before hybridization with the probe such that the higher-order structure of RNA can be degraded. Where the base strand of the nucleic acid probe is formed of 35 or fewer bases, addition of a helper probe, for example, an oligonucleotide the base sequence of which is (5')AGGCCGGCCCTTGACTTTCCT(3') to a reaction mixture is preferred for raising the efficiency of the hybridization to the sequence region. In this case, the helper probe can be in an oligodeoxyribonucleotide form or in a 2'-o-methyloligoribonucleotide form. When a nucleic acid probe longer than a 35-base strand is used, however, it is only necessary to thermally denature target RNA. When the nucleic acid probe according to the present invention is hybridized to RNA as described above, the fluorescence intensity decreases corresponding to the concentration of RNA in the reaction mixture, and RNA can be determined to a final RNA concentration of about 150 pM.

In determination of RNA by a conventional hybridization assay making use of a nucleic acid probe, an oligodeoxyribonucleotide or oligoribonucleotide has been used as the

nucleic acid probe. Because RNA itself has a higher-order solid structure, the efficiency of hybridization between the probe and the target RNA was poor, resulting in quantitation of low accuracy. The conventional methods, therefore, are

5 accompanied by irksomeness that a hybridization reaction is conducted after denaturing RNA and immobilizing denatured RNA on a membrane. The method according to the present invention, on the other hand, uses a nucleic acid probe a ribose portion of which has been modified to have high affinity to a particular

10 structural part of RNA, so that a hybridization reaction can be conducted at a higher temperature compared with the conventional methods. The above-mentioned adverse effects of the high-order structure of RNA can be overcome by simply conducting thermal denaturation as pretreatment and using a

15 helper probe in combination. As a consequence, the efficiency of hybridization in the method according to the present invention is practically as high as 100%, leading to improvements in the accuracy of quantitation. Further, the method according to the present invention is far simpler and

20 easier than the conventional methods.

The probe according to the present invention is formed of 5 to 50 bases, preferably 10 to 25 bases, most preferably 15 to 20 bases. A base number greater than 50 leads to lower permeability through a cell membrane when employed in a

25 fluorescent in situ hybridization assay, thereby narrowing an

000240 4213550

applicable range of the present invention. A base number smaller than 5, on the other hand, tends to induce non-specific hybridization and, therefore, results in a large determination error.

5           No particular limitation is imposed on the base sequence of the probe insofar as the probe hybridizes specifically to the target nucleic acid. Preferably, however, the base sequence of the probe may be designed such that, when the nucleic acid probe labeled with the fluorescent dye is hybridized with  
10           the target nucleic acid,

          (1) at least one G (guanine) base exists in the base sequence of the target nucleic acid at a position 1 to 3 bases apart from an end base portion where the probe and the target nucleic acid are hybridized with each other, or

15           (2) base pairs in a probe-nucleic acid hybrid complex form at least one G (guanine) and C (cytosine) pair at the end portion.

          The oligonucleotide in the nucleic acid probe in the present invention can be produced by a conventional production process for general oligonucleotides. It can be produced, for  
20           example, by a chemical synthesis process or by a microbial process which makes use of a plasmid vector, a phage vector or the like (Tetrahedron Letters, 22, 1859-1862, 1981; Nucleic Acids Research, 14, 6227-6245, 1986). Further, it is suitable to use a nucleic acid synthesizer currently available on the  
25           market (for example, "ABI394", trade name, manufactured by

000240 2295560

Perkin-Elmer Corp., Norwalk, Connecticut, U.S.A.).

To label the oligonucleotide with the fluorescent dye, desired one of conventionally-known labeling methods can be used (Nature Biotechnology, 14, 303-308, 1996; Applied and Environmental Microbiology, 63, 1143-1147, 1997; Nucleic Acids Research, 24, 4532-4535, 1996). To conjugate a fluorescent dye molecule to the 5' end, a spacer, for example,  $-(CH_2)_n-SH$  is first introduced into a phosphate group at the 5' end by a method known per se in the art. As such a spacer-introduced derivative is available on the market, a commercial product may be purchased (Midland Certified Reagent Company). In the above-mentioned example,  $n$  ranges from 3 to 8 with 6 being preferred. A labeled oligonucleotide can be synthesized by conjugating an SH-reactive fluorescent pigment or a derivative thereof with the spacer. The thus-synthesized oligonucleotide, which is labeled with the fluorescent dye, can be purified by reversed phase chromatography or the like to provide a nucleic acid probe for use in the present invention.

Further, the fluorescent dye can be conjugated to the 3' end of the oligonucleotide. In this case, a spacer, for example,  $-(CH_2)_n-NH_2$  is introduced onto an OH group on the C atom at the 3'-position of ribose or deoxyribose. As such a spacer-introduced derivative is also available on the market like the above-described ones, a commercial product may be purchased (Midland Certified Reagent Company). As an

000240-42795560



alternative, a phosphate group may be introduced, followed by the introduction of a spacer, for example,  $-(CH_2)_n-SH$  onto the OH group of the phosphate group. In these cases,  $n$  ranges from 3 to 8, with 4 to 7 being preferred. A labeled oligonucleotide can be synthesized by conjugating an amino- or SH-reactive fluorescent pigment or a derivative thereof with the spacer. The thus-synthesized oligonucleotide, which is labeled with the fluorescent dye, can be purified by reversed phase chromatography or the like to provide a nucleic acid probe for use in the present invention. For the introduction of the amino group, it is convenient to use a kit reagent [for example, "Unilink Aminomodifier" (trade name, product of Clontech Laboratories, Inc., Palo Alto, California, U.S.A.), or "FluoReporter Kit F-6082, F-6083, F-6084 or F-10220" (trade name, product of Molecular Probes, Inc.)]. In a manner known per se in the art, molecules of the fluorescent dye can then be conjugated to the oligoribonucleotide. It is also possible to introduce molecules of the fluorescent dye into strands of the probe nucleic acid (ANALYTICAL BIOCHEMISTRY, 225, 32-38, 1998).

The nucleic acid probe according to the present invention can be prepared as described above. A preferred probe form is one labeled with a fluorescent dye at the 3' or 5' end and containing G or C as the base at the labeled end. If the 5' end is labeled and the 3' end is not labeled, the OH group on the

invention is not limited to the determination of a nucleic acid, but it can also be suitably applied to methods for analyzing or determining polymorphism or mutation of a target nucleic acid or gene. In particular, its combined use with a DNA chip to be described subsequently herein provides a convenient method. Described specifically, the intensity of fluorescence upon hybridization of the nucleic acid probe of this invention with the target nucleic acid or gene varies depending on whether or not a GC pair is formed. It is, therefore, possible to analyze or determine polymorphism and/or mutation of a target nucleic acid or gene by hybridizing the nucleic acid probe according to the present invention to the target nucleic acid or gene and then measuring the intensity of emission. Specific methods will be described in Examples. In this case, the target nucleic acid or gene can be an amplified or extracted product obtained by desired one of nucleic acid or gene amplification or extraction methods. Further, no particular limitation is imposed on the kind of the target nucleic acid. Examples of the target nucleic acid to which the present invention is applicable can include RNAs, DNAs, PNAs, and artificially-modified nucleic acids. They are however required to contain

a guanine base in strands thereof or at ends thereof, because the intensity of fluorescence would otherwise not decrease. The method of the present invention can, therefore, analyze or determine a mutation or substitution such as G→A, G←A, C→T, C←T, G→C or G←C, specifically, polymorphism such as single nucleotide polymorphism (SNP). Incidentally, it is the current practice to perform an analysis of polymorphism by determining the base sequence of a nucleic acid or gene in accordance with the Maxam-Gilbert method or the dideoxy method.

Inclusion of the nucleic acid probe according to the present invention in a kit for analyzing or determining polymorphism and/or mutation of a target nucleic acid or gene, therefore, makes it possible to suitably use the kit as a kit for the analysis or determination of the polymorphism and/or mutation of the target nucleic acid or gene.

When analyzing data obtained by the method of the present invention for the analysis or determination of polymorphism and/or mutation of a target gene, a processing step may be added to correct the intensity of fluorescence, which is emitted from the reaction system when the target nucleic acid has hybridized to the nucleic acid probe labeled with the fluorescent dye, by the intensity of fluorescence emitted from the reaction system when the target nucleic acid and the nucleic acid probe have not hybridized with each other. The data so processed are provided with high reliability. Accordingly, the present

invention also provides a data analysis method for the method which analyzes or measures polymorphism and/or mutation of the target nucleic acid or gene.

The present invention also features a system for  
5 analyzing or determining polymorphism and/or mutation of a  
target nucleic acid or gene, which processing means for  
correcting a fluorescence intensity of a reaction system, in  
which the target nucleic acid or gene has hybridized to the  
nucleic acid probe labeled with the fluorescent dye, in  
10 accordance with a fluorescence intensity of the reaction system  
in which the target nucleic acid or gene has not hybridized to  
the nucleic acid probe labeled with the fluorescent dye.

The present invention further features a computer-readable recording medium with a program recorded therein for making a computer perform a processing step in which, when analyzing data obtained by the method for analyzing or determining polymorphism and/or mutation of a target nucleic acid or gene, a fluorescence intensity of a reaction system, in which the target nucleic acid or gene has hybridized to the nucleic acid probe labeled with the fluorescent dye, is corrected in accordance with a fluorescence intensity of the reaction system in which the target nucleic acid or gene has not hybridized to the nucleic acid probe labeled with the fluorescent dye.

25           The probe according to the present invention may be

immobilized on a surface of a solid (support layer), for example, on a surface of a slide glass. In this case, the probe may preferably be immobilized on the end not labeled with the fluorescent dye. The probe of this form is now called a "DNA chip". These DNA chips can be used for monitoring gene expressions, determining base sequences, analyzing mutations or analyzing polymorphisms such as single nucleotide polymorphism (SNP). Needless to say, they can also be used as devices (chips) for determining nucleic acids.

10 To bind the probe of the present invention, for example, to a surface of a slide glass, a slide glass coated with polycations such as polylysine, polyethyleneimine or polyalkylamine, a slide glass with aldehyde groups introduced thereon, or a slide glass with amino groups introduced thereon  
15 is first provided. Binding can then be achieved, for example, by i) reacting phosphate groups of the probe to the slide glass coated with the polycations, ii) reacting a probe, in which amino groups have been introduced, to the slide glass on which aldehyde groups have been introduced or iii) reacting a probe,  
20 in which PDC (pyridinium dichlornate) residual groups, amino groups or aldehyde groups have been introduced, to the slide glass on which amino groups have been introduced (Fodor, P.A., et al., Science, 251, 767-773, 1991; Schena, W., et al., Proc. Natl. Acad. Sci., U.S.A., 93, 10614-10619, 1996; McGal, G., et  
25 al., Proc. Natl. Acad. Sci., U.S.A., 93, 13555-13560, 1996;

Blanchad, A.P., et al., Biosens. Bioelectron., 11, 687-690, 1996).

5 A device having nucleic acid probes arranged and bound in an array form on a surface of a solid support permits more convenient determination of a nucleic acid.

10 In this case, formation of a device by individually binding many probes of this invention, the base sequences of which are different, on a surface of the same solid support makes it possible to simultaneously detect and quantitate a variety of genes.

15 Preferably, this device may be designed such that each probe is provided on a side of the solid support, said side being opposite to the side to which the probe is bound, with at least one temperature sensor and at least one heater and an area of the solid support, where the probe is bound, can be controlled to meet optimal temperature conditions.

20 For this device, probes other than those of the present invention, for example, nucleic acid probes of a construction designed such that two different fluorescent dyes are contained per molecule and each of the probes either quenches or emits fluorescence owing to interaction between the two fluorescent dyes when the probe is not hybridized with its corresponding target nucleic acid but either emits fluorescence or quenches when the probe hybridizes to the target nucleic acid,  
25 specifically, a device with molecular beacons described above

00555127-042000

(Tyagi et al., Nature Biotech., 14, 303-308, 1996) or the like bound thereon can also be used suitably. These devices, therefore, are embraced within the technical scope of the present invention.

5           Fundamental operations in the determination method making use of the device according to the present invention are simply to place a solution, which contains a target nucleic acid such as mRNA, cDNA or rRNA, on the solid support support on which the nucleic probes are bound and then to induce hybridization.  
10   As a result, a change in the intensity of fluorescence takes place corresponding to the concentration of the target nucleic acid, and the target nucleic acid can then be detected and quantitated from the change in the intensity of fluorescence. Further, binding of many nucleic acid probes of different base  
15   sequences on a surface of a single support makes it possible to detect and quantitate many nucleic acids at the same time. As this device can be used for exactly the same application as a DNA chip, it is a novel DNA chip. Under reaction conditions optimal for the target nucleic acid, the intensities of  
20   fluorescence emitted from the nucleic acids other than the target nucleic acid remain unchanged. No operation is, therefore, needed for washing off the unreacted nucleic acids. Further, independent temperature control of the individual nucleic acid probes by their corresponding microheaters makes  
25   it possible to control the probes under their optimal reaction

000240 219550

conditions, respectively. Accurate quantitation is therefore feasible. In addition, a dissociation curve between each nucleic acid probe and its corresponding target nucleic acid can be analyzed by continuously changing the temperature with the microheater and measuring the intensity of fluorescence during the changing of the temperature. From differences in such dissociation curves, it is possible to determine properties of the hybridized nucleic acid and also to detect SNP.

According to each conventional device for determining a concentrations of a target nucleic acid, a nucleic acid probe not modified with a fluorescent dye is bound or fixed on a surface of a solid support and, subsequent to hybridization with the target nucleic acid labeled with the fluorescent dye, an unhybridized portion of the target nucleic acid is washed off, followed by the measurement of the intensity of fluorescence from the remaining fluorescent dye.

To label the target nucleic acid with the fluorescent dye, the following steps can be followed, for example, when specific mRNA is chosen as a target: (1) mRNA extracted from cells is extracted in its entirety, and (2) using a reverse transcriptase, cDNA is synthesized while inserting a nucleoside modified by the fluorescent dye. These operations are not needed in the present invention.

A number of various probes are applied in spots on the



device. Optimal hybridization conditions, for example, temperatures or the like for nucleic acids to be hybridized to the individual probes are different from each other.

Theoretically speaking, it is therefore necessary to conduct  
5 a hybridization reaction and a washing operation under optimal conditions for each probe (at each spot). This is however physically impossible. For all the probes, hybridization is conducted at the same temperature and further, washing is also carried out at the same temperature with the same washing  
10 solution. The device is, therefore, accompanied by a drawback that a nucleic acid does not hybridize although its hybridization is desired or that, even if its hybridization takes place, the nucleic acid is readily washed off as the hybridization is not strong. For these reasons, the accuracy  
15 of quantitation of the nucleic acid is low. The present invention does not have such a drawback because the above-mentioned washing operation is not needed. Further, a hybridization reaction can be conducted at an optimal temperature for each probe by independently arranging a  
20 microheater at the bottom of each spot and controlling the hybridization temperature. Accordingly, the accuracy of quantitation has been significantly improved in the present invention.

In the present invention, use of the above-described  
25 nucleic acid probe or device makes it possible to specifically

determine a concentration of a target nucleic acid with ease in a short time.

A description will hereinafter be made of the determination method.

5 In the determination method according to the present invention, the above-described nucleic acid probe is added to a measurement system and is caused to hybridize to a target nucleic acid. This hybridization can be effected by a conventionally-known method (Analytical Biochemistry, 183,  
10 231-244, 1989; Nature Biotechnology, 14, 303-308, 1996; Applied and Environmental Microbiology, 63, 1143-1147, 1997). As conditions for hybridization, the salt concentration may range from 0 to 2 molar concentration, preferably from 0.1 to 1.0 molar concentration, and the pH may range from 6 to 8, preferably from  
15 6.5 to 7.5.

The reaction temperature may preferably be in a range of the  $T_m$  value of the hybrid complex, which is to be formed by hybridization of the nucleic acid probe to the specific site of the target nucleic acid,  $\pm 10^\circ\text{C}$ . This temperature range can  
20 prevent non-specific hybridization. A reaction temperature lower than  $T_m - 10^\circ\text{C}$  allows non-specific hybridization, while a reaction temperature higher than  $T_m + 10^\circ\text{C}$  allows no hybridization. Incidentally, a  $T_m$  value can be determined in a similar manner as in an experiment which is needed to design  
25 the nucleic acid probe for use in the present invention.

Described specifically, an oligonucleotide which is to be hybridized with the nucleic acid probe and has a complementary base sequence to the nucleic acid probe is chemically synthesized by the above-described nucleic acid synthesizer or the like, and the  $T_m$  value of a hybrid complex between the oligonucleotide and the nucleic acid probe is then measured by a conventional method.

The reaction time may range from 1 second to 180 minutes, preferably from 5 seconds to 90 minutes. If the reaction time is shorter than 1 second, a substantial portion of the nucleic acid probe according to the present invention remains unreacted in the hybridization. On the other hand, no particular advantage can be brought about even if the reaction time is set excessively long. The reaction time varies considerably depending on the kind of the nucleic acid, namely, the length or base sequence of the nucleic acid.

In the present invention, the nucleic acid probe is hybridized to the target nucleic acid as described above. The intensity of fluorescence emitted from the fluorescent dye is measured both before and after the hybridization, and a decrease in fluorescence intensity after the hybridization is then calculated. As the decrease is proportional to the concentration of the target nucleic acid, the concentration of the target nucleic acid can be determined.

The concentration of the target nucleic acid in the

reaction mixture may range from 0.1 to 10.0 nM, while the concentration of the probe in the reaction mixture may range from 1.0 to 25.0 nM. Upon preparation of a working curve, the probe may desirably be used at ratios of from 1.0 to 2.5 relative to the target nucleic acid.

Upon actually determining the concentration of a target nucleic acid, the concentration of which is unknown, in a sample, a working curve is first prepared under the below-described conditions. A corresponding probe is added at plural concentrations to aliquots of the sample, respectively, followed by the measurement of decreases in fluorescence intensity. The probe concentration, which corresponds to the greatest one of the decreases in fluorescence intensity so measured, is chosen as a preferred probe concentration. Based on the decrease in fluorescence intensity measured at the preferred probe concentration, a quantitated value of the target nucleic acid can be determined from the working curve.

A description has been made about the principle of the method of the present invention for the determination of a concentration of a nucleic acid. The present invention can be applied to various nucleic acid determination methods, for example, fluorescent *in situ* hybridization assays, PCR methods, ligase chain reactions, strand displacement assays, competitive hybridizations, and TAS methods led by the NASBA method.

Examples of these applications will hereinafter be described.

a) Application to fluorescent in situ hybridization assays

The present invention can be suitably applied to the determination of the concentration of a nucleic acid in cells of a cultivation system of microorganisms (e.g., a co-cultivation system of microorganisms or a symbiotic cultivation system of microorganisms), in which various kinds of microorganisms are contained together or a microorganism and other animal- or plant-derived cells are contained together and cannot be isolated from each other, or in a homogenate or the like of the cells of the cultivation system. The term "microorganisms" as used herein means microorganisms in general sense, and no particular limitation is imposed thereon.

Examples of such microorganisms can include eukaryotic microorganisms and prokaryotic microorganisms, and also mycoplasmas, virus and rickettsias. The term "a nucleic acid having a specific sequence" means a nucleic acid with a base sequence specific to cells of a cell strain which is desired to be investigated, for example, as to how it is acting in such a microorganism. Illustrative examples can include 5S rRNAs, 16S rRNAs and 23S rRNAs of certain specific cell strains and particular sequences of their gene DNAs.

According to the present invention, a nucleic acid probe is added to a co-cultivation system of microorganisms or a

000240 042000 0956127  
5 symbiotic cultivation system of microorganisms and the  
concentration of 5S rRNA, 16S rRNA or 23S rRNA of a particular  
cell strain or its gene DNA, thereby making it possible to  
determine the viable count of the particular strain in the  
10 system. Incidentally, a viable count of a particular cell  
strain in a co-cultivation system of microorganisms or a  
symbiotic cultivation system of microorganisms can be determine  
by adding the nucleic acid probe to a homogenate of the system  
and then measuring a decrease in fluorescence emission from the  
fluorescent dye before hybridization relative to fluorescence  
emission from the fluorescent dye after the hybridization. It  
is to be noted that this method also falls within the technical  
scope of the present invention.

15 The above-described determination method can be carried  
out as will be described hereinafter. Before the addition of  
the nucleic acid probe, the temperature, salt concentration and  
pH of the co-cultivation system of microorganisms or the  
symbiotic cultivation system of microorganisms are adjusted to  
meet the conditions described above. It is also preferable to  
20 adjust the concentration of the specific cell strain, which is  
contained in the co-cultivation system of microorganisms or the  
symbiotic cultivation system of microorganisms, to  $10^7$  to  $10^{12}$   
cells/mL, preferably  $10^9$  to  $10^{10}$  cells/mL in terms of viable count.  
These adjustments can be achieved by dilution, centrifugal or  
25 like concentration, or the like. A viable count smaller than

10<sup>7</sup> cells/mL results in low fluorescence intensity and greater determination error. A viable count greater than 10<sup>12</sup> cells/mL, on the other hand, leads to excessively high fluorescence intensity, so that the viable count of the particular  
5 microorganism cannot be determined quantitatively.

The concentration of the nucleic acid probe to be added depends upon the viable count of the particular cell strain in the co-cultivation system of microorganisms or the symbiotic cultivation system of microorganisms and, at a viable count of  
10 10<sup>8</sup> cells/mL, may be in a range of from 0.1 to 10.0 nM, preferably in a range of from 0.5 to 5 nM, more preferably 1.0 nM. A probe concentration lower than 0.1 nM cannot provide any data which accurately reflects the viable count of the particular  
15 microorganism. The probe concentration, however, cannot be specified in any wholesale manner because it depends upon the concentration of a target nucleic acid in cells.

Upon hybridizing the nucleic acid probe to the 5S rRNA, 16S rRNA or 23S rRNA of the particular cell strain or its gene DNA in the present invention, the reaction temperature may be  
20 set as described above. Further, the hybridization time may also be set as described above.

The nucleic acid probe is hybridized to the 5S rRNA, 16S rRNA or 23S rRNA of the particular cell strain or its gene DNA under such conditions as described above. A decrease in  
25 fluorescence emission from the fluorescent dye in the co-

cultivation system of microorganisms or the symbiotic cultivation system of microorganisms before the hybridization relative to the corresponding fluorescence emission before the hybridization is then determined.

5           The decrease in fluorescence emission from the florescent dye, which is determined as described above, is proportional to the viable count of the particular cell strain in the co-cultivation system of microorganisms or the symbiotic cultivation system of microorganisms, because the  
10           concentration of the 5S rRNA, 16S rRNA or 23S rRNA or its gene DNA and the viable count of the particular cell strain are proportional to each other.

          In the present invention, no particular limitation is imposed on components other than the microorganisms in the  
15           co-cultivation system of microorganisms or the symbiotic cultivation system of microorganisms, insofar as the components do not interfere with the hybridization between the nucleic acid probe according to the present invention and the 5S rRNA, 16S  
20           rRNA or 23S rRNA or its gene DNA and further, do not inhibit emission of fluorescence from the fluorescent dye in the nucleic acid probe. For example, phosphates such as  $\text{KH}_2\text{PO}_4$ ,  $\text{K}_2\text{HPO}_4$ ,  $\text{NaH}_2\text{PO}_4$  and  $\text{Na}_2\text{HPO}_4$ , inorganic nitrogen compounds such as ammonium sulfate, ammonium nitrate and urea, various salts of metal ions such as magnesium, sodium, potassium and calcium ions,  
25           various salts such as the sulfates, hydrochlorides, carbonates



and the like of trace metal ions such as magnesium, zinc, iron and cobalt ions, and vitamins may be contained to adequate extent. If the above-described interference or inhibition is observed, it may be necessary to separate cells of the plural  
5 microorganisms from the cultivation system by an operation such as centrifugal separation and then to resuspend them in a buffer or the like.

Usable examples of the buffer can include various buffers such as phosphate buffer, carbonate buffer, Tris-HCl buffer,  
10 Tris-glycine buffer, citrate buffer, and Good's buffer. The buffer should be adjusted to a concentration not inhibiting the hybridization, the FRET phenomenon or the emission of fluorescence from the fluorescent dye. This concentration depends upon the kind of the buffer. The pH of the buffer may  
15 range from 4 to 12, with 5 to 9 being preferred.

#### b) Application to PCR methods

The present invention can be applied to any method insofar as it is a PCR method. A description will hereinafter be made of an application of the present invention to a real-time  
20 quantitative PCR method.

In the real-time quantitative PCR method, PCR is conducted using a specific nucleic acid probe according to the present invention, and a decrease in fluorescence emission from the florescent dye before a reaction relative to fluorescence  
25 emission from the fluorescent dye after the reaction is

determined in real time.

The term "PCR" as used herein means a variety of PCR methods. Examples can include RT-PCR, RNA-primed PCR, stretch PCR, reverse PCR, PCR making use of an Alu sequence, multiple  
5 PCR, PCR making use of a mixed primer, and PCR making use of PNA. Further, the term "quantitative" means, in addition to quantitation in general sense, quantitation of such an extent as detection.

As described above, the term "target nucleic acid" as used  
10 herein means a nucleic acid the quantitation or qualitative detection or mere detection of which is intended, irrespective whether it is in a purified form or not and further irrespective of its concentration. Various other nucleic acids may also exist together with the target nucleic acid. For example, the  
15 target nucleic acid may be a specific nucleic acid in a co-cultivation system microorganisms (a mixed system of RNAs or gene DNAs of plural microorganisms) or a symbiotic cultivation system of microorganisms (a mixed system of RNAs or gene DNAs of plural animals, plants and/or microorganisms), the  
20 amplification of which is intended. Purification of the target nucleic acid, if needed, can be conducted by a method known per se in the art. For example, purification can be effected using a purification kit or the like available on the market.

The conventionally-known quantitative PCR methods  
25 individually amplify, in the presence of Mg ions, a target

nucleic acid by using dATP, dGTP, dCTP, dTTP or dUTP, a target nucleic acid (DNA or RNA), Taq polymerase, a primer, and a nucleic acid labeled with a fluorescent dye or an intercalator while repeatedly changing the temperature between low and high levels, and monitor increases in fluorescence emission from the fluorescent dye in real time in the course of the amplification [Jikken Igaku (Laboratory Medicine), 15(7), 46-51, Yodosha (1997)].

On the other hand, the quantitative PCR method according to the present invention is characterized in that the target nucleic acid is amplified by using the nucleic probe of the present invention and a decrease in fluorescence emission from the fluorescent dye is determined. The number of bases in a preferred probe of the present invention for use in the quantitative PCR according to the present invention may be from 5 to 50, preferably from 10 to 25, notably from 15 to 20. No particular limitation is imposed on the probe insofar as it hybridizes to amplification products of the target nucleic acid in PCR cycles. The probe may be designed in either a forward type or a reverse type.

The followings can be mentioned as illustrative examples:

(1) A probe labeled, at a 5' end portion, preferably, the 5' end thereof, with a fluorescent dye useful in the practice of the present invention. The base sequence of the probe is designed such that, when hybridized at the end portion with a

target nucleic acid, at least one G (guanine) base exists in the base sequence of the target nucleic acid at a position 1 to 3 bases apart toward the 5' side from the base on the 5' end at which the probe and the target nucleic acid are hybridized with each other.

(2) A probe similar to the probe (1) except that the 3' end is labeled with the fluorescent dye.

(3) A probe similar to the probe (1) except that the 3' end, for example, the OH group on the C atom at the 3'-position of ribose or deoxyribose at the 3' end has been modified by a phosphate group or the like or that the OH group at the 2'-position of ribose at the 3' end has been modified by a phosphate group or the like.

(4) A probe labeled at the 3' end portion, preferably the 3' end with the fluorescent dye useful in the practice of the present invention and containing G or C as a base at the 3' end.

(5) A probe similar to the probe (1) except that the 5' end portion, preferably, the 5' end is labeled with the fluorescent dye useful in the practice of the present invention.

(6) A probe labeled at the 5' end portion, preferably the 5' end with the fluorescent dye useful in the practice of the present invention and containing G or C as a base at the 5' end.

In the case of each of the probes (4), (6), the 5' end may not be designed to G or C due to the base sequence of a target nucleic acid. If this should be the case, 5'-guanylic acid or

5'-cytidylic acid may be added to the 5' end of an oligonucleotide designed as a primer from the base sequence of the target nucleic acid. The probe so obtained can still achieve the objects of the present invention adequately. The expression "nucleic acid probe designed such that the 3' end or 5' end base thereof becomes G or C" as used herein is, therefore, defined to embrace not only probes designed based on the base sequence of the target nucleic acid but also probes added at the 3' end or 5' end thereof with 5'-guanylic acid or 5'-cytidylic acid.

In particular, the above-described probe (1), (2), (3) or (4) is designed such that it is not used as a primer. PCR is conducted by using a single probe of the present invention as opposed to two (fluorescent-dye-labeled) probes needed in a real-time quantitative PCR method making use of the FRET phenomenon. The probe is added to a PCR reaction system, and PCR is then conducted. During a nucleic acid extending reaction, the probe which has been in a form hybridized with the target nucleic acid or amplified target nucleic acid is degraded by polymerase and is dissociated off from the hybrid complex. The intensity of fluorescence of the reaction system at this time or the reaction system in which a nucleic acid denaturing reaction has completed is measured. Further, the intensity of fluorescence of the reaction system in which the target nucleic acid or amplified target nucleic acid has hybridized with the

probe (i.e., the reaction system at the time of an annealing reaction or at the time of the nucleic acid extending reaction until the probe is eliminated from the hybrid complex by polymerase). By calculating a decrease of the latter

5 fluorescence intensity from the former fluorescence intensity, the concentration of the amplified nucleic acid is determined. The intensity of fluorescence is high when the probe has completely dissociated from the target nucleic acid or

10 amplified target nucleic acid by the nucleic acid denaturing reaction or when the probe has been degraded out from the hybrid complex of the probe and the target nucleic acid or amplified nucleic acid at the time of extension of the nucleic acid. However, the intensity of fluorescence of the reaction system in which an annealing reaction has been completed and the probe

15 has fully hybridized to the target nucleic acid or amplified target nucleic acid or of the reaction system until the probe is degraded out of the hybrid complex of the probe and the target nucleic acid or amplified target nucleic acid by polymerase at the time of a nucleic acid extending reaction is lower than the

20 former. The decrease in the intensity of fluorescence is proportional to the concentration of the amplified nucleic acid.

In this case, each of the base sequences of the probes (2), (3), (4) may desirably be designed such that the  $T_m$  of a

25 hybrid complex, which is available upon hybridization of the

probe with the target nucleic acid, falls within a range of the  $T_m$  value of the hybrid complex of the primer  $\pm 15^\circ\text{C}$ , preferably  $\pm 5^\circ\text{C}$ . If the  $T_m$  of the probe is lower than (the  $T_m$  value of the primer  $- 5^\circ\text{C}$ ), especially (the  $T_m$  value of the primer  $- 15^\circ\text{C}$ ), the probe does not hybridize so that no decrease takes place in the fluorescence emission from the fluorescent dye. If the  $T_m$  of the probe is higher than (the  $T_m$  value of the primer  $+ 5^\circ\text{C}$ ), especially (the  $T_m$  value of the primer  $+ 15^\circ\text{C}$ ), the probe also hybridizes to nucleic acid or acids other than the target nucleic acid so that the specificity of the probe is lost.

The probes (5), (6) are added as primers to PCR reaction systems. Except for the PCR method according to the present invention, no PCR method is known to make use of a primer labeled with a fluorescent dye. As the PCR reaction proceeds, the amplified nucleic acid is progressively labeled with the fluorescent dye useful in the practice of the present invention. Accordingly, the intensity of fluorescence of the reaction system in which the nucleic acid denaturing reaction has completed is high but, in the reaction system in which the annealing reaction has completed or the nucleic acid extending reaction is proceeding, the intensity of fluorescence of the reaction system is lower than the former intensity of fluorescence.

The PCR reaction can be conducted under similar conditions as in conventional PCR methods. It is, therefore,

possible to conduct amplification of a target nucleic acid in a reaction system the concentration of Mg ions in which is low (1 to 2 mM). Needless to say, the present invention can also be conducted even in a reaction system in which Mg ions are  
5 contained at such a high concentration (2 to 4 mM) as that employed in the conventionally-known quantitative PCR methods.

In the PCR method according to the present invention,  $T_m$  value can be determined by conducting the PCR of the present invention and then analyzing the melting curve of the nucleic  
10 acid with respect to the amplification products. This method is a novel analysis method of a melting curve of a nucleic acid. In this method, the nucleic acid probe employed as a nucleic acid probe or primer in the PCR method of the present invention can be used suitably.

15 In this case, designing of the base sequence of the probe according to the present invention into a sequence complementary with a region containing SNP (single nucleotide polymorphism) makes it possible to detect SNP from a difference, if any, in a dissociation curve of the nucleic acid from the  
20 probe of the present invention by analyzing the dissociation curve after completion of PCR. If a base sequence complementary with an SNP-containing sequence is used as a sequence for the probe of the present invention, a  $T_m$  value available from a dissociation curve between the sequence of the probe and the  
25 SNP-containing sequence becomes higher than a  $T_m$  value

000240 22195560



available from a dissociation curve between the sequence of the probe and the SNP-free sequence.

A second feature of the present invention resides in the method for analyzing data obtained by the above-described  
5 real-time quantitative PCR method.

A real-time quantitative PCR method is now practiced in real time by a system which is composed of a reactor for conducting PCR, an equipment for detecting fluorescence emission from a fluorescent dye, a user interface, namely, a  
10 computer-readable recording medium with various procedures of a data analysis method recorded as a program (also called "sequence detection software system), and a computer for controlling them and analyzing data. Determination by the present invention is also conducted by such a system.

15 A description will first be made of an analyzer for real-time quantitative PCR. Any system can be used in the present invention insofar as it can monitor PCR in real time. Particularly suitable examples can include "ABI PRISM™ 7700 Sequence Detection System (SDS 7700)" (manufactured by  
20 Perkin-Elmer Applied Biosystems, Inc., U.S.A.) and "LightCycler™ System" (manufactured by Roche Diagnostics, Mannheim, Germany).

The above-described reactor is an apparatus for repeatedly conducting a thermal denaturing reaction of a target  
25 nucleic acid, an annealing reaction and an extending reaction

of the nucleic acid (these reactions can be repeatedly conducted, for example, by successively changing the temperature to 95°C, 60°C and 72°C. The detection system comprises a fluorescence emitting argon laser, a spectrograph and a CCD camera. Further, the computer-readable recording medium with the various procedures of the data analysis method recorded as the program is used by installing it in the computer, and contains a program recorded therein for controlling the above-described system via the computer and also for processing and analyzing data outputted from the detection system.

The data analysis program recorded in the computer-readable recording medium comprises the following steps: measuring the intensity of fluorescence cycle by cycle, displaying each measured fluorescence intensity as a function of cycles, namely, as a PCR amplification plot on a display of the computer, calculating a threshold cycle number (Ct) at which the intensity of fluorescence is begun to be detected, forming a working line useful in determining from Ct values the number of copies of the nucleic acid in the sample, and printing data and plot values in the respective steps. When PCR is exponentially proceeding, a linear relationship is established between the logarithm of the number of copies of the target nucleic acid at the time of initiation of PCR and Ct. It is therefore possible to calculate the number of copies of the target nucleic acid at the time of initiation of PCR by forming

a working line based on known copy numbers of the target nucleic acid and detecting the Ct of a sample which contains the target nucleic acid the number of copies of which is unknown.

5 The PCR-related invention is an invention for analyzing data obtained by such a real-time quantitative PCR method as described above. Its respective features will be described hereinafter.

10 A first feature resides in a processing step for correcting a fluorescence intensity of a reaction system, which is measured when the nucleic acid amplified in each cycle is conjugated with the fluorescent dye or when the amplified nucleic acid hybridizes to a nucleic acid probe labeled with the fluorescent dye in the method for analyzing data obtained by the real-time quantitative PCR method, by a fluorescence  
15 intensity of the reaction system as obtained when the above-described conjugate or hybrid complex has dissociated in each cycle, namely, the first feature resides in a correction-processing step.

20 As a specific example of "the reaction system ..... when the nucleic acid amplified in each cycle is conjugated with the fluorescent dye or when the amplified nucleic acid hybridizes to a nucleic acid probe labeled with the fluorescent dye", a reaction system upon conducting a nucleic acid extending reaction or annealing at 40 to 85°C, preferably 50 to 80°C in  
25 each cycle of PCR can be mentioned. The actual temperature

00556427.042000

depends upon the length of the amplified nucleic acid.

Further, "the reaction system ..... when the above-described conjugate or hybrid complex has dissociated" can be a reaction system upon conducting thermal denaturation of the nucleic acid in each cycle of PCR, specifically at a reaction temperature of from 90 to 100°C, preferably 94 to 96°C.

Any correction processing can be used as the correction processing in the correction processing step insofar as it conforms with the objects of the present invention. Specifically, correction processing including a processing step by the following formula (1) or formula (2) can be exemplified.

$$f_n = f_{\text{hyb},n} / f_{\text{den},n} \quad (1)$$

$$f_n = f_{\text{den},n} / f_{\text{hyb},n} \quad (2)$$

where

$f_n$ : correction-processed value in an  $n^{\text{th}}$  cycle as calculated in accordance with the formula (1) or formula (2),

$f_{\text{hyb},n}$ : intensity value of fluorescence of the reaction system available after the amplified nucleic acid has conjugated to the fluorescent dye or the amplified nucleic acid has hybridized to the nucleic acid probe labeled with the fluorescent dye in the  $n^{\text{th}}$  cycle, and

$f_{\text{den},n}$ : intensity value of fluorescence of the reaction system available after the nucleic acid-fluorescent dye

conjugate has dissociated in the  $n^{\text{th}}$  cycle.

This step includes a sub-step in which correction-processed values obtained by the above-described processing are displayed on a computer display and/or are printed or the  
5 correction-processed values are likewise displayed and/or printed in the form of a graph as a function of cycles.

A second feature resides in a data analysis method, which comprises:

10 introducing correction-processed values, which have been calculated in accordance with the formula (1) or formula (2) in individual cycles, into the following formula (3) or formula (4) to calculate rates or percentages of changes in fluorescence between samples in the individual cycles:

$$F_n = f_n / f_s \quad (3)$$

$$F_n = f_s / f_n \quad (4)$$

where

$F_n$ : rate or percentage of a change in fluorescence in an  $n^{\text{th}}$  cycle as calculated in accordance with the formula (3) or formula (4),

20  $f_n$ : correction-processed value calculated in the  $n^{\text{th}}$  cycle as calculated in accordance with the formula (1) or formula (2), and

$f_s$ : correction-processed value calculated in a given cycle before a change in  $f_n$  is observed as calculated in  
25 accordance with the formula (1) or formula (2), and in

general, a correction-processed value, for example, in one of 10<sup>th</sup> to 40<sup>th</sup> cycles, preferably one of 15<sup>th</sup> to 30<sup>th</sup> cycles, more preferably one of 20<sup>th</sup> to 30<sup>th</sup> cycles is adopted; and

5 comparing the rates or percentages of changes in fluorescence.

This step includes a sub-step in which calculated values obtained by the above-described processing are displayed on a computer display and/or are printed or the calculated values are likewise displayed and/or printed in the form of a graph as a function of cycles. This sub-step may be applied or may not be applied to the correction-processed values obtained by the formula (1) or formula (2).

10 A third feature resides in a data analysis method, which comprises the following processing steps:

15 1) performing processing in accordance with the following formula (5), (6) or (7) by using data of rates or percentages of changes in fluorescence as calculated in accordance with said formula (3) or (4):

$$20 \quad \log_b(F_n), \ln(F_n) \quad (5)$$

$$\log_b\{(1-F_n) \times A\}, \ln\{(1-F_n) \times A\} \quad (6)$$

$$\log_b\{(F_n-1) \times A\}, \ln\{(F_n-1) \times A\} \quad (7)$$

where

A, b: desired numerical values, preferably integers, more preferably natural numbers and, when A=100, b=10,  $\{(F_n-1)$

x A} is expressed in terms of percentage (%), and

$F_n$ : rate or percentage of a change in fluorescence in an  $n^{\text{th}}$  cycle as calculated in accordance with the formula (3) or formula (4),

5        2) determining a cycle in which said processed value of said processing step 1) has reached a constant value,

10        3) calculating a relational expression between cycle of a nucleic acid sample of a known concentration and the number of copies of said target nucleic acid at the time of initiation of a reaction, and

4) determining the number of copies of said target nucleic acid in an unknown sample upon initiation of PCR.

Preferably, these steps are performed in the order of 1) → 2) → 3) → 4).

15        Each of these steps 1) to 3) includes a sub-step in which processed values obtained by the corresponding processing are displayed on a computer display and/or are printed or the processed values are likewise displayed and/or printed in the form of a graph as a function of cycles. The step 4) should  
20        include at least a printing sub-step as the processed values obtained in the step 4) have to be printed, although the processed values obtained in the step 4) may also displayed on a computer display.

25        Incidentally, the correction-processed values obtained by the formula (1) or (2) and the calculated values obtained

by the formula (3) or (4) may be or may not be displayed on a computer display and/or printed in the form of graphs as a function of cycles, respectively. These displaying and/or printing sub-steps may, therefore, be added as needed.

5           The above-described data analysis method is particularly effective when decreases in fluorescence emission from the fluorescent dye are measured in the real-time quantitative PCR method. As a specific example, the real-time quantitative PCR method according to the present invention can be mentioned.

10           A fourth feature resides in an analysis system for real-time quantitative PCR, which comprises processing and storing means for performing a data analysis method for the above-described real-time quantitative PCR method of the present invention.

15 A fifth feature resides in a computer-readable recording medium with individual procedures of a data analysis method, which is adapted to analyze PCR by using the analysis sytem for the real-time quantitative PCR, stored as a program therein, wherein the program is designed to make a computer perform the  
20 individual procedures of the data analysis method of the present invention.

A sixth feature resides in a novel method for determining a nucleic acid, which comprises using the data analysis method, determination and/or analysis system and/or recording medium of the present invention in the nucleic acid determination



method.

A seventh feature resides in a method for analyzing data obtained by the above-described method of the present invention for the analysis of a melting curve of a nucleic acid, namely, data obtained by the method of the present invention in which the  $T_m$  value of the nucleic acid is determined by conducting PCR.

Specifically, the seventh feature resides in an analysis method, which comprises the following steps: gradually heating a nucleic acid, which has been amplified by the PCR method of the present invention, from a low temperature until complete denaturation of the nucleic acid (for example, from 50°C to 95°C; measuring an intensity of fluorescence at short time intervals (for example, at intervals equivalent to a temperature rise of from 0.2°C to 0.5°C) during the heating step; displaying results of the measurement as a function of time on a display, namely, a melting curve of the nucleic acid; differentiating the melting curve to obtain differentiated values ( $-dF/dT$ , F: intensity of fluorescence, T: time); displaying the differentiated values as derivatives on the display; and determining a point of inflection from the derivatives. In the present invention, the intensity of fluorescence increases as the temperature rises. Preferable results can be obtained in the present invention by adding to the above-described step a further processing step in which in each cycle, the intensity of fluorescence at the

time of the nucleic acid extending reaction, preferably at the time of completion of the PCR reaction is divided by the value of fluorescence intensity at the time of the thermal denaturing reaction.

5           A measurement and/or analysis system for the real-time quantitative PCR of the present invention, said real-time quantitative PCR including the method of the present invention for the analysis of the melting curve of a nucleic acid to the above-described novel method of the present invention for the  
10       analysis of data obtained by a PCR method, also falls within the technical scope of the present invention.

          A still further feature of the present invention resides in a computer-readable recording medium with the individual procedures of the method of the present invention for the  
15       analysis of the melting curve of a nucleic acid recorded therein as a program such that the procedures can be performed by a computer or a computer-readable recording medium with the individual procedures of the method of the present invention for the analysis of data obtained by a PCR method recorded  
20       therein as a program such that the procedures can be performed by a computer, wherein a program designed to make the computer perform the individual procedures of the method of the present invention for the analysis of the melting curve of the nucleic acid is additionally recorded.

25           The above-described data analysis methods, systems and

000040" 225550

recording media of the present invention can be used in a variety of fields such as medicine, forensic medicine, anthropology, paleontology, biology, genetic engineering, molecular biology, agricultural science and phytobreeding. They can be suitably applied to microorganism systems called "co-cultivation systems of microorganisms" or "symbiotic cultivation systems of microorganisms", in each of which various kinds of microorganisms are contained together or a microorganism and other animal- or plant-derived cells are contained together and cannot be isolated from each other. The term "microorganisms" as used herein means microorganisms in general sense, and no particular limitation shall be imposed thereon. Illustrative are eukaryotic microorganisms, prokaryotic microorganisms, mycoplasmas, virus and rickettsias.

The vial count of a particular cell strain in a co-cultivation system of microorganisms or a symbiotic cultivation systems of microorganisms can be determined by determining the number of copies of the 5S rRNA, 16S rRNA or 23S rRNA of the particular cell strain or its gene DNA in the system by using one or more of the above-described data analysis methods, systems and recording media of the present invention, because the number of copies of the gene DNA of 5S rRNA, 16S rRNA or 23S rRNA is specific to each cell strain. In the present invention, the vial count of a particular cell strain can also be determined by applying the real-time quantitative PCR of the

present invention to a homogenate of a co-cultivation system of microorganisms or a symbiotic cultivation systems of microorganisms. It shall also be noted that this method also falls with the technical scope of the present invention.

5           The present invention will next be described more specifically based on the following Examples and Comparative Examples.

#### Example 1

10           Preparation of a nucleic acid probe to be hybridized to the base sequence of a nucleic acid ranging from the 335<sup>th</sup> base to 358<sup>th</sup> base counted from the 5' end in 16S rRNA of *Escherichia coli*, namely, preparation of a nucleic acid probe having a base sequence of (3')CCGCTCACGCATC(5') was conducted as will be described hereinafter.

#### 15   Preparation of nucleic acid probe

          A deoxyribooligonucleotide, which had the base sequence of (3')CCGCTCACGCATC(5') and contained  $-(CH_2)_7-NH_2$  bonded to the OH group on the carbon atom at the 3' position of deoxyribose at the 3' end of the deoxyribooligonucleotide, was purchased from Midland Certified Reagent Company, U.S.A. From Molecular Probes, Inc., "FluoroReporter Kit F-6082" (trade name) was also purchased, which contained not only "BODIPY FL" propionic acid succinimidyl ester but also a reagent for conjugating the compound to the amine derivative of the oligonucleotide. The  
20           kit was caused to act on the above-purchased oligonucleotide,  
25

whereby a nucleic acid probe labeled with "BODIPY FL" was synthesized for use in this Example.

Purification of synthesized product

The synthesized product was dried into a dry product. The dry product was dissolved in 0.5 M  $\text{NaHCO}_3/\text{Na}_2\text{CO}_3$  buffer (pH 9.0). The solution was subjected to gel filtration through "NAP-25 Column" (trade name, product of Pharmacia AB, Uppsala, Sweden), whereby unreacted substances were removed. Further, reversed phase HPLC (B gradient: 15 to 65%, 25 minutes) was conducted under the below-described conditions. An eluted main fraction was collected. The collected fraction was lyophilized, whereby a nucleic acid probe was obtained with a yield of 23% as calculated relative to 2 mM of the starting oligonucleotide.

The above-described reversed phase chromatography was conducted under the following conditions:

Eluting solvent A: 0.05 N TEAA 5%  $\text{CH}_3\text{CN}$

Eluting solvent B (for gradient elution): 0.05 N TEAA  
40%  $\text{CH}_3\text{CN}$

Column: CAPCEL PAK C18 (trade name), 6 x 250 mm

Elution rate: 1.0 mL/min

Temperature: 40°C

Detection: 254 nm

Example 2

Using a 200-mL Erlenmeyer flask which contained sterilized nutrient broth (NB) (50 mL; product of Difco;

composition: NB, 0.08 g/100 mL), *Escherichia coli* JM109 was cultured overnight at 37°C under shaking. To the culture, an equivalent amount of 99.7% ethanol was then added. A 2-mL aliquot of the ethanol-added culture was centrifuged in a 2.0-mL Eppendorf centrifuge tube, whereby cells were obtained. The cells were washed once with 30 mM phosphate buffer (sodium salt) (100  $\mu$ L; pH 7.2). The cells were suspended in the phosphate buffer (100  $\mu$ L) which contained 130 mM NaCl. The suspension was ultrasonicated for 40 minutes under ice cooling (output: 33 W, oscillating frequency: 20 kHz, oscillation method: 0.5-second oscillation, followed by a 0.5-second pause), whereby a homogenate was prepared.

After the homogenate was centrifuged, the supernatant was collected and was then transferred into a cell of a fluorimeter. The cell with the supernatant placed therein was controlled at 36°C. A solution of the above-described nucleic acid probe, said solution having had been controlled to 36°C beforehand, was added to the supernatant to give a final concentration of 5 nM. While controlling at 36°C, *E. coli* 16S rRNA and the nucleic acid probe were hybridized for 90 minutes. Intensity of fluorescence emission from the fluorescent dye was then measured by the fluorimeter.

As the intensity of fluorescence emission from the fluorescent dye before the hybridization, a value measured by using 30 mM phosphate buffer (sodium salt), which contained 130

000240" 2219550

mM NaCl, (pH: 7.2) instead of the above-described supernatant was adopted. Intensity of fluorescence emission was measured by changing the ratio of the amount of the nucleic probe to the amount of the supernatant (exciting light: 503 nm; measured  
5 fluorescence color: 512 nm). The results are shown in FIG. 1. As is appreciated from FIG. 1, the intensity of fluorescence emission from the fluorescent dye decreased as the ratio of the amount of the supernatant increased. Namely, it is understood that in the present invention, the magnitude of a decrease in  
10 fluorescence emission from a fluorescent dye becomes greater in proportion to the amount of a target nucleic acid to which a nucleic acid probe hybridizes.

### Example 3

#### Preparation of nucleic acid probe

15 An oligonucleotide, which was to be hybridized to 23S rNA of *Escherichia coli* JM109, had a base sequence of (5') CCCACATCGTTTTGTCTGGG(3') and contained  $-(CH_2)_7-NH_2$  bonded to the OH group on the carbon atom at the 3' position of the 5' end nucleotide of the oligonucleotide, was purchased from  
20 Midland Certified Reagent Company, U.S.A. as in Example 1. From Molecular Probes, Inc., "FluoroReporter Kit F-6082" (trade name) was also purchased, which contained not only "BODIPY FL" propionic acid succinimidyl ester but also a reagent for conjugating the compound to the amine derivative of the  
25 oligonucleotide. The kit was caused to act on the above-

purchased oligonucleotide, whereby a nucleic acid probe labeled with "BODIPY FL" was synthesized. The synthesized product so obtained was purified as in Example 1, whereby the nucleic acid probe labeled with "BODIPY FL" was obtained with a yield of 25% as calculated relative to 2 mM of the starting oligonucleotide.

5

#### Example 4

With *Escherichia coli* JM109 cells obtained in Example 2, cells of *Pseudomonas paucimobilis* (now called "*Sphingomonas paucimobilis*) 421Y (FERM P-5122), said cells having have been obtained using the same culture medium and cultivation conditions as in Example 2, were mixed at the same concentration as *Escherichia coli* JM109 in terms of OD660 value, whereby a co-cultivation system of the microorganisms was prepared. From the resulting mixed system in which the cell concentration of *Escherichia coli* JM109 was the same as that in Example 2, a homogenate was prepared in the same manner as in Example 2. An experiment was conducted in a similar manner as in Example 2 except that the nucleic acid probe prepared in Example 3 was used, 543 nm exciting light was used, and 569 nm fluorescence was measured. The results were similar to those obtained in Example 2.

10

15

20

#### Example 5

The base selectivity of a target nucleic acid in the quenching phenomenon fluorescence, that is, the base selectivity according to the present invention was investigated.

25

000040 2219560



Ten kinds of synthetic deoxyribooligonucleotides (30 mer; poly a to poly j), which will be described subsequently herein, were prepared by a DNA synthesizer, "ABI394" (trade name; manufactured by Perkin-Elmer Corp.)

5 Also prepared were the below-described probes according to the present invention, which were labeled with "BODIPY FL" at the 5' ends of deoxyribooligonucleotides corresponding to the above-described synthetic DNAs, respectively.

10 Primer DNAs, which corresponded to the above-described synthetic DNAs and contained  $-(CH_2)_6-NH_2$  bonded to the phosphate groups at the 5' ends of the primer DNAs, were purchased from Midland Certified Reagent Company. From Molecular Probes, Inc., "FluoroReporter Kit F-6082" (trade name) was also  
15 purchased, which contained not only "BODIPY FL" propionic acid succinimidyl ester but also a reagent for conjugating the compound to the amine derivative of the oligonucleotide. The kit was caused to act on the above-purchased primer DNAs, whereby invention nucleic acid probes labeled with "BODIPY FL" (probes a, b, c, d, f, g, h) were synthesized. An investigation  
20 was made under the below-described conditions to determine how much the fluorescence emission from the fluorescent dye would decrease when the probes were caused to hybridize to their corresponding synthetic deoxyribooligonucleotides, and the specificity of the invention probes was studied.

000240" 2219550

	<u>Name</u>	<u>Target deoxyribooligonucleotide</u>
	poly a	5' ATATATATTTTTTTTTTGTTTTTTTTTTTTTT3'
	poly b	5' ATATATATTTTTTTTTTGTTTTTTTTTTTTTT3'
	poly c	5' ATATATATTTTTTTTTTGTTTTTTTTTTTTTT3'
5	poly d	5' ATATATATTTTTTTTTTGTTTTTTTTTTTTTT3'
	poly e	5' ATATATATTTTTTTTTTGTTTTTTTTTTTTTT3'
	poly f	5' ATATATATTTTTTTTTCTTTTTTTTTTTTTTT3'
	poly g	5' ATATATATTTTTTTTTCTTTTTTTTTTTTTTT3'
	poly h	5' ATATATATTTTTTTTTCTTTTTTTTTTTTTTT3'
10	poly i	5' ATATATATTTTTTTTTCTTTTTTTTTTTTTTT3'
	poly j	5' ATATATATTTTTTTTTCTTTTTTTTTTTTTTT3'
	<u>Name</u>	<u>Invention probe</u>
	Probe a	3' TATATATAAAAAAAAAACAA5' -BODIPY FL/C6
	Probe b	3' TATATATAAAAAAAAAACA5' -BODIPY FL/C6
15	Probe c	3' TATATATAAAAAAAAAAC5' -BODIPY FL/C6
	Probe d	3' TATATATAAAAAAAAAAA5' -BODIPY FL/C6
	Probe f	3' TATATATAAAAAAAAAAGAA5' -BODIPY FL/C6
	Probe g	3' TATATATAAAAAAAAAAGA5' -BODIPY FL/C6
	Probe h	3' TATATATAAAAAAAAAAG5' -BODIPY FL/C6

20 (1) Components of hybridization mixture

Synthetic DNA	320 nM (final concentration)
Nucleic acid probe	80 nM (final concentration)
NaCl	50 nM (final concentration)
MgCl <sub>2</sub>	1 nM (final concentration)
25 Tris-HCl buffer (pH 7.2)	100 nM (final concentration)

70

"MilliQ" purified water 1.6992 mL

Final whole volume 2.0000 mL

(2) Hybridization temperature: 51°C

(3) Measuring conditions

5 Exciting light: 543 nm

Measured fluorescence color: 569 nm

Table 1

Nucleic acid probe	Target nucleic acid	Decrease in Fluorescence intensity (%)
a	a	-10
b	b	2
c	c	75
d	d	48
d	e	18
f	f	-8
g	g	-2
h	h	70
d	i	-6
d	j	-5

10 The results are shown in Table 1. As is appreciated from Table 1, it is preferred to design the base sequence of a nucleic acid probe labeled with a fluorescent dye such that, when the nucleic acid probe is hybridized with a target DNA

000240 22795560

(deoxyribooligonucleotide), at least one G (guanine) base exists in the base sequence of the target DNA at a position 1 to 3 bases apart from an end base portion where the probe and the target DNA are hybridized with each other. From Table 1, it is also understood to be desired to design the base sequence of a nucleic acid probe labeled with a fluorescent dye such that, when the nucleic acid probe is hybridized with a target, base pairs in the probe-DNA hybrid complex form at least one G (guanine) and C (cytosine) pair at the end portion.

#### Example 6

Target nucleic acids and invention nucleic acid probes of the below-described base sequences were prepared. In a similar manner as in the preceding Example, an investigation was made about effects of the number of G(s) in each target nucleic acid and the number of G(s) in its corresponding invention nucleic acid probe.

72

Name Target deoxyribooligonucleotide

	poly k	5' TATATATATATATTTTGGGGG3'
	poly l	5' TATATATATATATTTTGGGGG3'
	poly m	5' TATATATATATTTTTTTTGGGG3'
5	poly n	5' TATATATATTTTTTTTTTGGG3'
	poly o	5' TATATATATTTTTTTTTTGG3'
	poly p	5' TATATATATATTTTCCCCC3'
	poly q	5' TATATATATATTTTCCCCC3'
	poly r	5' TATATATATTTTTTTTCCC3'
10	poly s	5' TATATATATTTTTTTTCC3'
	poly t	5' TATATATATTTTTTTTTC3'
	poly u	5' TATATATATTTTTTTTTT3'

Name Invention probe

15	probe k	3' ATATATATATAAAAAACCCCC5' -BODIPY FL/C6
	probe l	3' ATATATATATAAAAAACCCCC5' -BODIPY FL/C6
	probe m	3' ATATATATATAAAAAAACCC5' -BODIPY FL/C6
	probe n	3' ATATATATATAAAAAAAACC5' -BODIPY FL/C6
	probe o	3' ATATATATATAAAAAAAAAC5' -BODIPY FL/C6
20	probe p	3' ATATATATATAAAAAAGGGGG5' -BODIPY FL/C6
	probe q	3' ATATATATATAAAAAAGGGG5' -BODIPY FL/C6
	probe r	3' ATATATATATAAAAAAAGGG5' -BODIPY FL/C6
	probe s	3' ATATATATATAAAAAAAGG5' -BODIPY FL/C6
	probe t	3' ATATATATATAAAAAAAG5' -BODIPY FL/C6
25	probe u	3' ATATATATATAAAAAAAA5' -BODIPY FL/C6

000240-2219550

Table 2

Nucleic acid probe	Target nucleic acid	Decrease in Fluorescence intensity (%)
k	k	93
l	l	92
m	m	94
n	n	92
o	o	87
p	p	61
q	q	68
r	r	69
s	s	75
t	t	73
u	u	2

As is appreciated from Table 2, neither the number of G(s) in a target nucleic acid nor the number of G(s) in an invention probe substantially affects a decrease in fluorescence intensity.

#### Example 7

Target nucleic acids and invention nucleic acid probes of the below-described base sequences were prepared. In a similar manner as in the preceding Example, an investigation was made about effects of the kind of bases in each target nucleic

acid and the kind of bases in its corresponding invention nucleic acid probe.

	<u>Name</u>	<u>Target deoxyribooligonucleotide</u>
	poly W	5'CCCCCCTTTTTTTTTTTT3'
5	poly X	5'GGGGGGAATAAAAAAAAAA3'
	poly Y	5'TTTTTTCCCCCCCCCCCC3'
	poly Z	5'AAAAAGGGGGGGGGGGG3'

	<u>Name</u>	<u>Invention probe</u>
10	probe w	BODIPY FL/C6-5'AAAAAAAAGGGGGG3'
	probe x	BODIPY FL/C6-5'TTTTTTTTCCCCCC3'
	probe y	BODIPY FL/C6-5'GGGGGGGGGAATAA3'
	probe z	BODIPY FL/C6-5'CCCCCCCCTTTTTT3'

000240" 2295560

75

Table 3

Nucleic acid probe	Target nucleic acid	Fluorescence intensity from probe alone (A)	Fluorescence intensity after addition of target nucleic acid (B)	Decrease in fluorescence intensity, % (C)*
W	w	330	380	-15
X	x	440	430	2
Y	y	40	50	25
Z	z	360	30	92

\* Decrease in fluorescence intensity, % (C) =  $\{(A-B)/A\} \times 100$

000240" 22799560



As is appreciated from Table 3 and the preceding Example, a substantial decrease takes place in fluorescence intensity (i) when an end of an invention probe labeled with a fluorescent dye is composed of C and hybridization of a target nucleic acid forms a G-C pair, or (ii) when an end of an invention probe labeled with a fluorescent dye is composed of a base other than C and at least one G exists on a side closer to the 3' end of a target nucleic acid than a base pair formed of a base at a location where the invention probe is labeled with the fluorescent dye and a base of the target nucleic acid.

#### Example 8

Concerning the kinds of dyes usable for labeling nucleic acid probes of the present invention, an investigation was made in a similar manner as in the preceding Examples. As an invention probe, the probe z of Example 7 was used. As a target nucleic acid, on the other hand, the oligonucleotide z of Example 7 was employed.

The results are shown in Table 4. As is readily envisaged from this table, illustrative fluorescent dyes suitable for use in the present invention can include FITC, "BODIPY FL", "BODIPY FL/C3", 6-joe, and TMR.

77

Table 4

Fluorescent dye	Decrease in fluorescence intensity (%)
FITC	90
"BODIPY FL"	95
"BODIPY FL/C3"	98
"BODIPY FL/C3"	97
6-joe	75
TMR	93

Incidentally, the decreases (%) in fluorescence intensity were calculated in a similar manner as in Example 7.

Example 9

Preparation of nucleic acid probe

An oligonucleotide was purchased from Midland Certified Reagent Company, U.S.A. as in Example 1. The oligonucleotide had a base sequence of

(5')CATCCCCACCTTCCTCCCAGTTGACCCCGGCAGTC(3') (35 base pairs) hybridizable specifically to the 16S rRNA base sequence of KYM-7 strain, said base sequence being equivalent to the base sequence ranging from the 1156<sup>th</sup> base to the 1190<sup>th</sup> base of the 16S rRNA of *Escherichia coli* JM109, contained deoxyribonucleotides at the 1<sup>st</sup> to 16<sup>th</sup> bases and the 25<sup>th</sup> to 35<sup>th</sup> bases, respectively, said methyl-modified ribonucleotides being modified with methyl groups at the OH group at the 2'position on the carbon atom or ribose, and was modified with  $-(CH_2)_7-NH_2-$  at the

phosphate group of the 5'-terminal group of the 35 base pairs. From Molecular Probes, Inc., "FluoroReporter Kit F-6082" (trade name) was also purchased, which contained not only "BODIPY FL/C6" propionic acid succinimidyl ester but also a reagent for  
5 conjugating the compound to the amine derivative of the oligonucleotide. The kit was caused to act on the above oligonucleotide, whereby a nucleic acid probe labeled with "BODIPY FL/C6" was synthesized. The synthesized product so obtained was purified as in Example 1, whereby the nucleic acid  
10 probe labeled with "BODIPY FL/C6" was obtained with a yield of 23% as calculated relative to 2 mM of the starting oligonucleotide. This probe was named "35-nucleotides-chained 2-O-Me probe".

Using a DNA synthesizer, a riboxyligoligonucleotide having  
15 a base sequence of (5')AGGCCGGCCCTTGACTTTCCT(3') was synthesized as in the above to provide it as a forward-type hepter probe. On the other hand, a riboxyligoligonucleotide having a base sequence of  
(5')AUGGGAGUUCAGUAGUACCCGCAUUGCUGGUCC(3') was synthesized by  
20 using a DNA synthesizer, thereby providing it as a reverse-type helper probe.

The above-described 16S rRNA was subjected to heat treatment at 95°C for 5 minutes, and was then added to a probe solution which had been maintained under the below-described  
25 reaction conditions. By a fluorescence measuring instrument

“Perkin-Elmer LS-50B” (trade name), the intensity of fluorescence was measured. The results are shown in FIG. 2. Incidentally, data obtained by using 16S rRNA which was not subjected to the above-described heat treatment are plotted as a control. It is understood from FIG. 2 that substantial decreases in fluorescence intensity took place in the experimental group in the experimental group subjected to heat treatment. These results indicate that heat treatment of 16S rRNA at 95°C induces stronger hybridization with the probe according to the present invention.

Reaction conditions:

16S rRNA:	10.0 nm
Probe:	25 nM
Buffer:	100 mM succinic acid, 125 mM lithium hydroxide, 8.5% lithium dodecylsulfite, pH 5.1
Temperature:	70°C

Example 10

Effects of helper probe on the efficiency of hybridization

Invention probes and helper probes, which were to be hybridized to the above-described 16S rRNA, were prepared in a similar manner as described above. Under conditions to be described subsequently herein, an investigation was made about effects of a 2'-O-Me probe of the present invention, effects

of the length of a nucleotides chain in the probe and effects of a helper probe. The results are presented in diagrams A, B, C and D in FIG. 3. It is appreciated from these diagrams that the 2'-O-Me probe according to the present invention contributes to the efficiency of hybridization. It is also understood that the helper probe is effective in increasing the efficiency of hybridization when the base strand of the 2'-O-Me probe is short.

1) The same 35-nucleotides-chained 2'-O-Me probe as described above.

2) A probe having the same base sequence as the 35-nucleotides-chained 2'-O-Me described above under 1) except that the oligonucleotide is formed of a deoxyribonucleotide (33-nucleotides-chained DNA probe).

3) A probe having the same base sequence as the 35-nucleotides chained 2'-O-Me described above under 1) except that the nucleotides ranging over 8 bases from the 5' end and 16 bases from the 3' end were removed (17-nucleotides-chained 2-O-Me probe).

4) A probe having the same base sequence as the 33-nucleotides-chained 2-O-Me probe described above under 2) except that a nucleotide ranging over 16 bases from the 3' end was removed (17-nucleotides-chained DNA probe).

5) A helper probe obtained by modifying the OH groups of the central 8 bases of the above-described forward-type helper

probe with methyl groups (forward-type 2-O-Me-helper probe).

6) A helper probe obtained by modifying the OH groups of the central 8 bases of the above-described reverse-type helper probe with methyl groups (reverse-type 2-O-Me-helper probe).

5 7) A helper probe having the same base sequence as the above-described forward helper probe except that the oligonucleotide is formed of a deoxyribonucleotide (forward-type DNA helper probe).

10 8) A helper probe having the same base sequence as the above-described reverse helper probe except that the oligonucleotide is formed of a deoxyribonucleotide (reverse-type DNA helper probe).

15 9) A ribooligonucleotide having a base sequence of 5') GUGACGGUCACUAUUUGACCUCCUCCACCCC (3') (35-base ribooligonucleotide).

10) A ribooligonucleotide having a base sequence of 5') GUGACGGUCACUAUUUG (3') (17-base ribooligonucleotide).

Reaction conditions:

20	Concentration of 16S rRNA:	10 nM
	Concentration of probe:	25 nM
	Helper probe concentration:	1 $\mu$ M
25	Buffer composition:	100 mM succinic acid, 125 mM lithium hydroxide, 8.5% lithium dodecyl- sulfite, pH 5.1

## Reaction temperature:

70°C (for 35-nucleotides-chained 2-O-Me probe)

65°C (for 17-nucleotides-chained 2-O-Me probe and  
33-nucleotides-chained DNA probe)

5 50°C (for 17-nucleotides-chained DNA probe)

## Example 12

## Preparation of working curve for rRNA determination

At diverse concentrations within a range of from 0.1 to 10 nM, the above-described rRNA was heated at 95°C for 5 minutes.

10 The resulting nucleic acid solutions were added to aliquots of a reaction mixture, respectively. The reaction mixture had been prepared and maintained under the below-described reaction conditions. Upon elapsed time of 1,000 seconds, decreases in fluorescence intensity were measured using "Perkin-Elmer

15 LS-50B". The results are plotted in FIG. 4. It is appreciated from the diagram that the working curve shows linearity in the range of from 0.1 to 10 nM.

## Reaction conditions:

Concentrations of 33-nucleotides-

20 chained 2-O-Me probe: 10 nM

Buffer composition: 100 mM succinic acid,  
125 mM lithium hydroxide,  
8.5% lithium dodecyl-  
sulfite, pH 5.1

25 Reaction temperature: 70°C

## Example 12

## Florescent in situ hybridization assay

In a similar manner as described above, 35-nucleotides-chained 2-O-Me probe and 36-nucleotides-chained 2-O-Me probe according to the present invention were prepared for hybridization to the respective rRNAs of *Cellulomonas* sp. KYM-7 (FERM P-16806) and *Agrobacterium* sp. KYM-8 (FERM P-11358), respectively. Those probes had the following base sequences:

35-nucleotides-chained 2-O-Me probe for assaying the rRNA of *Cellulomonas* sp. KYM-7:

(5') CATCCCCACCTTCCTC CGAGTTGA CCCCCGGCAGTC (3')

(the boxed bases are modified with methyl groups)

36-nucleotides-chained 2-O-Me probe for assaying the rRNA of *Agrobacterium* sp. KYM-8:

(5') CATCCCCACCTTCCTC TCGGCTTAT CACCGGCAGTC (3')

(the boxed bases are modified with methyl groups)

*Cellulomonas* sp. KYM-7 (FERM P-16806) and *Agrobacterium* sp. KYM-8 (FERM P-11358) were co-cultured with the below-described medium composition under the below-described cultivation conditions. Co-cultures were sampled at various phases of the co-cultivation. From each of the co-cultures, rRNAs were prepared using "RNeasy Maxikit" (trade name; product of QIAGEN GmbH (Hilden, Germany)). Those rRNAs were heated at 95°C for 5 minutes, and then added to the reaction mixture which had been maintained under the reaction conditions. After they



were reacted at 70°C for 1,000 seconds, a decrease in fluorescence intensity was measured using "Perkin-Elmer LS-50B". The results are plotted in FIG. 5. Incidentally, the total rRNA was measured using "RiboGreen RNA Kit" (trade name; product of Molecular Probe, Inc. (Eugene, Oregon, U.S.A.)).

As is appreciated from the diagram, the mobilizations of the rRNAs of the respective cell strains were consistent with that of the total rRNA. This indicates that the method of the present invention can be effectively used in fluorescent in situ hybridization assays.

Composition of culture medium (g/L):

Starch, 10.0; aspartic acid, 0.1 ;  $K_2HPO_4$ , 5.0;  $KH_2PO_4$ , 5.0;  $KH_2PO_4$ , 2.0;  $MgSO_4 \cdot 7H_2O$ , 0.2; NaCl, 0.1;  $(NH_4)_2SO_4$ , 0.1.

Cultivation conditions:

The above-describe cell strains were cultivated beforehand on a slant medium. One roopful of the culture was collected from the slant medium, and was then inoculated to the above-described sterilized nutrient broth (NB) in an Erlenmeyer flask. The strains were cultured at 30°C and 150 rpm under shaking.

Reaction conditions:

Concentrations of 33-nucleotides-

chained 2-O-Me probe: 1.0 to 10 nM

Buffer composition: 100 mM succinic acid,

125 mM lithium hydroxide,  
8.5% lithium dodecyl-  
sulfite, pH 5.1

Reaction temperature: 70°C

5 A method for analyzing polymorphism and mutation of a  
target nucleic acid or gene will hereinafter be described in  
Example 13.

#### Example 13

000240 22195560  
10 Four oligonucleotides with the below-described base  
sequences were synthesized using the same DNA synthesizer as  
that employed in Example 5. Further, an invention nucleic acid  
probe having the below-described base sequence was also  
synthesized in a similar manner as in Example 5. The  
15 oligonucleotides were separately hybridized with the probe in  
solutions. An investigation was then made as to whether or not  
a single base substitution can be determined from a change in  
fluorescence intensity. The base sequence of the nucleic acid  
probe according to the present invention is designed such that,  
20 if G exists at the 3' end of any one of the target oligonucleotides,  
it matches 100% with the base sequence of the particular  
oligonucleotide. The hybridization temperature was set at 40°C  
at which all base pairs between the probe and the target  
oligonucleotide can hybridize 100%. The concentrations of the  
probe and target oligonucleotides, the concentration of a  
25 buffer solution, a fluorimeter, fluorescence measuring

conditions, experimental procedures, and the like were set or chosen as in Example 5.

Invention probe: 3'TTTTTTTTGGGGGGGGC5'BODIPY FL/C6

Target nucleotide No. 1: 5'AAAAAAAACCCCCCCCCA3'

5 Target nucleotide No. 2: 5'AAAAAAAACCCCCCCCC3'

Target nucleotide No. 3: 5'AAAAAAAACCCCCCCCCI3'

(I: hypoxanthine)

Target nucleotide No. 4: 5'AAAAAAAACCCCCCCCCG3'

10 The results are shown in Table 5. As is appreciated from the table, no change in fluorescence intensity was observed in the case of the target oligonucleotides Nos. 1 to 3, but in the case of the target oligonucleotide No. 4, a decrease as much as 84% was observed.

15

Table 5

Target oligo-nucleotide	Initial fluorescence intensity (A)	Fluorescence intensity after hybridization (B)	(A-B)/B
No. 1	340	350	-0.03
No. 2	332	328	0.01
No. 3	343	336	0.02
No. 4	345	52	0.84

In the method of the present invention for analyzing data (for example, the data in columns A and B in Table 5) obtained

by the method for analyzing or determining polymorphism and/or mutation of a target nucleic acid or gene (for example, the target oligonucleotide No. 1, 2, 3 or 4), the processing to correct a fluorescence intensity of a reaction system, said  
5 fluorescence intensity being obtained when a target nucleic acid or gene is hybridized with a nucleic acid probe labeled with a fluorescent dye (for example, the above-described nucleic acid probe), by a fluorescence intensity of the same reaction system when the target nucleic acid or gene is not  
10 hybridized with the nucleic acid probe means the calculation of  $(A-B)/B$  in Table 3.

From the above results, it has been found that, when a target nucleic acid is a double-stranded nucleic acid, substitutions of  $G \rightarrow A$ ,  $G \leftarrow A$ ,  $C \rightarrow T$ ,  $C \leftarrow T$ ,  $G \rightarrow C$  and  $G \leftarrow C$  can be  
15 detected.

#### Example 14

A model of A DNA chip according to the present invention is illustrated in FIG. 6. Firstly, a modified probe and a surface-treated slide glass are provided first. The modified  
20 probe had been prepared by introducing an amino group onto the 3'-OH group at the 3' end of the invention probe, 3' TTTTTTTTGGGGGGGC5' BODIPY FL/C6, prepared in Example 13. On the other hand, the surface-treated slide glass had been prepared by treating a slide glass with a silane coupling agent  
25 which contained epoxy groups as reactive groups. A solution

00000 " 0429560

with the modified probe contained therein was applied in spots onto the surface-treated slide glass by a DNA chip production apparatus, "GMS™ 417 ARRAYER" (manufactured by TAKARA SHUZO CO., LTD., Kyoto, Japan). As a result, the modified probe is bound at the 3' end onto a surface of the slide glass. The slide glass is then placed for 4 hours or so in a closed vessel to bring the reaction to completion. The slide glass was alternately dipped in 0.1% SDS solution and water, twice in each of the solution and water, for about 1 minute each time. Further, the slide glass was immersed for about 5 minutes in a boron solution, which had been prepared by dissolving  $\text{NaBH}_4$  (1.0 g) in water (300 mL). Shortly after the slide glass was placed for 2 minutes in water of 95°C, the slide glass was alternately dipped in 0.1% SDS solution and water, twice in each of the solution and water, for about 1 minute each time, so that reagents were washed off. The slide glass was then dried. As a result, a DNA chip according to the present invention was prepared.

Further, arrangement of a minute temperature sensor and a microheater on the lower side of the slide glass at a position corresponding to each spot of the modified probe makes it possible to provide the DNA chip of the present invention with high performance.

A description will next be made of a determination of a target nucleic acid or gene by the DNA chip. No change takes

place in fluorescence intensity where the target nucleic acid or gene is not hybridized with the probe, where no G-C pair is formed at the fluorescent-dye-labeled end even if they are hybridized together, or where at least one G (guanine) base does not exist in the base sequence of the target nucleic acid or gene at a position 1 to 3 bases apart from an end base portion where the probe and the target nucleic acid or gene are hybridized with each other. However, the intensity of fluorescence decreases when hybridization takes place. This fluorescence intensity can be measured by using a DNA chip analyzer, "GMS™ 418 Array Scanner" (manufactured by TAKARA SHUZO CO., LTD.).

Methods of the present invention for PCR assay will hereinafter be described in Examples 15-19.

#### Example 15

Using as a target nucleic acid the 16S rRNA gene in the genome DNA of *Escherichia coli*, a primer labeled with "BODIPY FL/C6) was prepared for the amplification of the nucleic acid.

#### Preparation of Primer 1 (Eu800R: reverse type)

A deoxyribooligonucleotide having a base sequence of (5')CATCGTTTACGGCGTGGAC(3') was synthesized using a DNA synthesizer, "ABI394" (trade name; manufactured by Perkin-Elmer, Corp.). An oligonucleotide, which had been prepared by treating the phosphate group at the 5'end of the oligodeoxyribonucleotide with phosphatase to form cytosine and

then bonding  $-(CH_2)_9-NH_2$  to the OH group on the carbon atom at the 5'-position of the cytosine, was purchased from Midland Certified Reagent Company. From Molecular Probes, Inc., "FluoroReporter Kit F-6082" (trade name) was also purchased, which contained not only "BODIPY FL" propionic acid succinimidyl ester but also a reagent for conjugating the compound to the amine derivative of the oligonucleotide. The kit was caused to act on the above-purchased oligonucleotide, whereby Primer 1 of the present invention labeled with "BODIPY FL/C6" was synthesized.

#### Purification of synthesized product

The synthesized product was dried into a dry product. The dry product was dissolved in 0.5 M  $Na_2CO_3/NaHCO_3$  buffer (pH 9.0). The solution was subjected to gel filtration through "NAP-25 Column" (trade name, product of Pharmacia AB, Uppsala, Sweden), whereby unreacted substances were removed. Further, reversed phase HPLC (B gradient: 15 to 65%, 25 minutes) was conducted under the below-described conditions. An eluted main fraction was collected. The collected fraction was lyophilized, whereby Primer 1 of the present invention was obtained with a yield of 50% as calculated relative to 2 mM of the starting oligonucleotide.

The above-described reversed phase chromatography was conducted under the following conditions:

Eluting solvent A: 0.05 N TEAA 5%  $CH_3CN$

Eluting solvent B (for gradient elution): 0.05 N TEAA

40% CH<sub>3</sub>CN

Column: CAPCEL PAK C18 (trade name), 6 x 250 mm

Elution rate: 1.0 mL/min

5 Temperature: 40°C

Detection: 254 nm

#### Example 16

##### Preparation of Primer 2 (Eu500R/forward: forward type)

10 Primer 2 composed of a deoxyribooligonucleotide, which had a base sequence of (5')CCAGCAGCCGCGGTAATAC(3'), and a fluorescent dye ("BODIPY FL/C6") labeled to the 5' end of the deoxyribooligonucleotide, was prepared with a yield of 50% in a similar manner as in Example 13.

#### Example 17

15 Using a test tube containing a liquid culture medium (5 mL; composition: NB, 0.08 g/100 mL) of sterilized nutrient broth (NB) (product of Difco), *Escherichia coli* JM109 was cultivated overnight at 37°C under shaking. A 1.5-mL aliquot of the culture was centrifuged in a 1.5-mL centrifuge tube, 20 whereby cells were obtained. From the cells, genome DNA was extracted using "DNeasy Tissue Kit" (trade name, product of QIAGEN GmbH, Hilden, Germany). The extraction was conducted following the protocol of the kit. As a result, a 17-ng/μL DNA solution was obtained.



## Example 18

Using the genome DNA of the above *E. coli* strain, Primer 1 and/or Primer 2, PCR reactions were conducted by a method known per se in the art while using "LightCycler™ System" (trade name) marketed from Roche Diagnostics, Mannheim, Germany.

Operations were conducted following the manual of the system.

In the above system, PCR was conducted as specified in the manual except that Primer 1 and/or Primer 2 of the present invention were used in place of nucleic acid probes (two nucleic acid probes making use of the FRET phenomenon) and a general primer (a general primer not labeled with any fluorescent dye), both of which are listed in the manual).

PCR was conducted in a hybridization mixture of the following components:

15	<i>E. coli</i> genome DNA solution	3.5 $\mu$ L
	(final concentration: 0 to 6 ng/20 $\mu$ L)	
	(final copy number: 0 to $2.4 \times 10^6$ copies)	
	Primer solution	0.8 $\mu$ L
	(final concentration: 0.08 $\mu$ M)	
20	Taq solution	10.0 $\mu$ L
	"MiliQ" purified water	5.7 $\mu$ L
	Final whole volume	20.0 $\mu$ L

Incidentally, the experiments were conducted by using the target nucleic acid, *E. coli* 16S rDNA, at the concentrations of the respective experimental groups shown in the brief

description of FIG. 7 and also by using the primers in the combinations of Primer 1 and/or Primer 2 also shown in the brief description of FIG. 7.

The above Taq solution is a mixed solution of the following reagents:

Taq solution	96.0 $\mu$ L
"MiliQ" purified water	68.2 $\mu$ L
Taq DNA polymerase solution	24.0 $\mu$ L
Taq start	3.8 $\mu$ L

Incidentally, these Taq solution and Taq DNA polymerase solution were both included in the "DNA Master Hybridization Probe Kit" (trade name; product of Roche Diagnostics, Mannheim, Germany). Specifically, as the Taq DNA polymerase solution, the 10 x conc. solution (red cap) was used by diluting it tenfold. Further, Taq start is an antibody for the Taq DNA polymerase and is marketed by Clontech Laboratories, Inc., Palo Alto, California, U.S.A. Addition of Taq start to a reaction mixture can suppress activity of Taq DNA polymerase up to 70°C.

The following reaction conditions were used.

Denaturation	Initial: 95°C, 120 seconds
	Second and onwards: 95°C, 120 seconds
Annealing	57°C, 5 seconds

Measurements were conducted using "LightCycler™ System" (manufactured by Roche Diagnostics, Mannheim Germany). For each measurement, the detector F1 was used out of the detectors

F1-F3 included in the system, and the gain and excitation level of the detector were set at 10 and 75, respectively.

The results are shown in FIG. 7 and FIG. 8. It is appreciated from FIG. 7 and FIG. 8 that the number of cycles at the time of observation of a decrease in fluorescence emission from the fluorescent dye and the number of copies of *E. coli* 16S rDNA as the target nucleic acid are proportional to each other. In these diagrams, decreases in fluorescence emission from the fluorescent dye are expressed in terms of decreases in the intensity of fluorescence.

FIG. 9 shows a working line for *E. coli* 16S rDNA, in which the number of copies of *E. coli* 16S rDNA is expressed as a function of cycles. The correlation coefficient was 0.9973, so that extremely good correlation was exhibited.

As is understood from the above results, use of the quantitative PCR method of the present invention makes it possible to count the number of copies of a target nucleic acid at the beginning. This means that the concentration of the target nucleic acid can be determined.

#### Example 19

In Example 18, PCR was conducted using the invention probes as primers. In this example, however, PCR according to the present invention was conducted under the following conditions by using a primer of the present invention as opposed to two probes required in the conventional method making use

of the FRET phenomenon.

a) Target nucleic acid: 16S rDNA of *Escherichia coli*

b) Primers:

- Forward primer E8F: (3')AGAGTTTGATCCTGGCTCAG(5')

- Reverse primer E1492R: GGTTACCTTGTTACGACTT(5')

c) Probe: BODIPY FL-(3')CCTTCCCACATCGTTT(5')

d) PCR apparatus: "LightCycler™ System" (manufactured  
by Roche Diagnostics, Mannheim  
Germany)

e) Conditions for PCR:

Denaturation: 95°C for 0 second

(95°C for 60 seconds in the  
first cycle only)

Annealing: 50°C for 5 seconds

Extension: 72°C for 70 seconds

Total cycle number: 70 cycles

f) Fluorescence assay (measurement):

Assay (measurement) was performed once after each of  
denaturation and annealing in each cycle.

g) Composition of reaction mixture:

Total volume: 20 µL

Amount of DNA polymerase ("TaKaRa Ex taq"): 0.5 U

Amount of TaqStart antibody: 0.3 µL

Concentration of primer: 0.2 µM (common to both  
primers)

Concentration of probe: 0.05  $\mu$ M

Concentration of  $MgCl_2$ : 2 mM

Conc. of BSA (bovine serum albumin): 0.25 mg/mL

Concentration of dNTPs: 0.2 mM (for each nucleotide)

5           The results are shown in FIG. 10. It is understood from the diagram that the number of cycles at the time of observation of a decrease in fluorescence emission from the fluorescent dye and the number of copies of *E. coli* 16S rDNA as the target nucleic acid are proportional to each other.

10           As is understood from the above results, use of the quantitative PCR method of the present invention makes it possible to count the number of copies of a target nucleic acid at the beginning. This means that the concentration of the target nucleic acid can be determined.

15           In the subsequent Examples, the data analysis method of the present invention for analyzing data obtained by using the above-described quantitative PCR method of the present invention will be described.

#### Example 20

20           Using, as a target nucleic acid, human genome DNA (human  $\beta$ -globin) (TaKara Catalog Product No. 9060) (product of TAKARA SHUZO CO., LTD., Kyoto Japan) (hereinafter called "the human genome DNA"), a primer labeled with "BODIPY FL/C6" was prepared for the amplification of the nucleic acid.

000240 0435560

Preparation of Primer KM38+C (reverse type)

A deoxyribooligonucleotide having a base sequence of (5')CTGGTCTCCTTAAACCTGTCTTG(3') was synthesized using a DNA synthesizer, "ABI394" (trade name; manufactured by Perkin-Elmer, Corp.). An oligonucleotide, which had been prepared by treating the phosphate group at the 5' end of the oligodeoxyribonucleotide with phosphatase to form cytosine and then bonding  $-(CH_2)_6-NH_2$  to the OH group on the carbon atom at the 5'-position of the cytosine, was purchased from Midland Certified Reagent Company. From Molecular Probes, Inc., "FluoroReporter Kit F-6082" (trade name) was also purchased, which contained not only "BODIPY FL" propionic acid succinimidyl ester but also a reagent for conjugating the compound to the amine derivative of the oligonucleotide. The kit was caused to act on the above-purchased oligonucleotide, whereby Primer KM38+C of the present invention labeled with "BODIPY FL/C6" was synthesized.

Purification of synthesized product

The synthesized product was dried into a dry product. The dry product was dissolved in 0.5 M  $Na_2CO_3/NaHCO_3$  buffer (pH 9.0). The solution was subjected to gel filtration through "NAP-25 Column" (trade name, product of Pharmacia AB, Uppsala, Sweden), whereby unreacted substances were removed. Further, reversed phase HPLC (B gradient: 15 to 65%, 25 minutes) was conducted under the below-described conditions. An eluted main fraction

was collected. The collected fraction was lyophilized, whereby Primer KM38+C of the present invention was obtained with a yield of 50% as calculated relative to 2 mM of the starting oligonucleotide.

- 5           The above-described reversed phase chromatography was conducted under the following conditions:

Eluting solvent A: 0.05 N TEAA 5% CH<sub>3</sub>CN

Eluting solvent B (for gradient elution): 0.05 N TEAA  
40% CH<sub>3</sub>CN

- 10           Column: CAPCEL PAK C18 (trade name), 6 x 250 mm  
Elution rate: 1.0 mL/min  
Temperature: 40°C  
Detection: 254 nm

Example 21

- 15           Preparation of Primer KM29 (forward type)

A deoxyribooligonucleotide having a base sequence of (5')GGTTGGCCAATCTACTCCCAGG(3') was synthesized in a similar manner as in Example 18.

Comparative Example 1

- 20           This Comparative Example is directed to use of a data analysis software which did not include the processing step of the present invention that an intensity of fluorescent during an extending reaction of a nucleic acid is divided using an intensity of fluorescent at the time of a thermal denaturing  
25           reaction [i.e., the processing of the formula (1)].

Using the above-described human genome DNA, Primer KM38+C and Primer KM29, PCR reactions were conducted by "LightCycler™ System" (manufactured by Roche Diagnostics, Mannheim Germany). The intensity of fluorescence was measured in each cycle.

5           Incidentally, the PCR in this Comparative Example employed the above-described primers labeled with the fluorescent dye, and is a novel real-time quantitative PCR method in which a decrease in fluorescence emission is measured rather than an increase in fluorescence emission. Analysis of  
10           data was conducted using the software of the system itself. The PCR in this Comparative Example was conducted following the manual of the system except that the invention primers KM38+C and KM29 were used instead of the nucleic acid probes listed in the (two probes making use of the FRET phenomenon) or an  
15           ordinary primer (an ordinary primer not labeled with any fluorescent dye).

PCR was conducted in a hybridization mixture of the following components:

20	Human genome DNA	1.0 $\mu\text{L}$
	(final concentration: 1 to 10,000 copies)	
	Primer solution	4.0 $\mu\text{L}$
	(final concentration: 0.1 $\mu\text{M}$ )	
	Taq solution	10.0 $\mu\text{L}$
	"MiliQ" purified water	5.0 $\mu\text{L}$
25	Final whole volume	20.0 $\mu\text{L}$



Incidentally, the experiments were conducted by using the human genome at the concentrations of the respective experimental groups shown in the brief description of FIG. 11.

The following reaction conditions were used.

- 5      Denaturation      Initial: 95°C, 60 seconds  
                            Second and onwards: 95°C, 10 seconds  
            Annealing      60°C, 5 seconds  
            DNA extending reaction: 72°C, 17 seconds

- 10      Measurements were conducted using "LightCycler™ System" (manufactured by Roche Diagnostics, Mannheim Germany). For each measurement, the detector F1 was used out of the detectors F1-F3 included in the system, and the gain and excitation level of the detector were set at 10 and 75, respectively.

- 15      PCR was conducted as described above, during which the intensities of fluorescence in individual cycles were measured. The results are shown in FIG. 11. Described specifically, with respect to each of the human genome DNAs of the respective copy numbers, the intensity of fluorescence was measured at the time of a denaturing reaction and also at the time of a nucleic acid  
20      extending reaction, both in each cycle, and was printed. It is observed that the intensity of fluorescence remained constant at the time of the denaturing reaction irrespective of the cycle but a decrease in fluorescence took place from the 25th cycle at the time of the nucleic acid extending reaction.  
25      It is also understood that this decrease occurs earlier as the

number of copies of the human genome DNA increases.

As is shown in FIG. 11, the intensities of fluorescence in initial cycles were not constant irrespective of the number of copies of the human genome DNA. The following steps (b)-(i) were, therefore, added to the data analysis method for use in this Comparative Example.

(b) Assuming that the intensity of fluorescence in the 10<sup>th</sup> cycle is 1, the intensity of fluorescence in each cycle is converted, namely, calculation is conducted in accordance with the following formula (8):

$$C_n = (72)/F_{10}(72) \quad (8)$$

where

$C_n$ : converted value of the intensity of fluorescence in each cycle,

$F_n(72)$ : the intensity of fluorescence after extending reaction at 72°C in each cycle, and

$F_{10}(72)$ : the intensity of fluorescence in the 10<sup>th</sup> cycle.

(c) Each converted value obtained in step (b) is displayed on a display and/or printed as a function of cycle.

(d) From the converted value in each cycle as obtained in step (b), the rate of a change in fluorescence intensity (decrease or quench, %) is calculated in accordance with the following formula (9):

$$F_{dn} = \log \{100 - C_n \times 100\} \quad (9)$$

$$F_{dn} = 2 \log \{1 - C_n\} \quad (9)$$

000240 429550

where

$F_{dn}$ : the rate of a change in fluorescence intensity  
(decrease or quench, %), and

5  $C_n$ : the value obtained in accordance with the formula  
(8).

(e) Each converted value obtained in step (d) is displayed  
on a display and/or printed as a function of cycle.

10 (f) Data processed in step (d) are compared with 0.5 as a  
threshold, and the number of cycles the data of which reach the  
threshold is counted.

(g) A graph is prepared by plotting values, which have been  
counted in step (f), along X-axis and the numbers of copies  
before the initiation of the reaction along Y-axis.

15 (h) The graph prepared in step (g) is displayed on a display  
or printed.

(i) A correlation coefficient or relational formula of the  
line drawn in step (h) is calculated.

20 (j) The correlation coefficient or relational formula  
calculated in step (i) is displayed on a display or printed.

Using the above-described data analysis software, the  
data obtained in FIG. 11 were then processed as will be described  
hereinafter.

FIG. 12 is a print-out of the data processed in step (b)  
25 [process (c)]. Namely, assuming that the intensity of

000040" 2279560

fluorescence in the 10<sup>th</sup> cycle was 1, the fluorescence intensities in the individual cycles were converted, and the converted values were plotted against the corresponding cycles.

FIG. 13 is a print-out of the data processed in step (d) [process (e)]. Namely, decreases (%) (quenches, %) of the respective fluorescence intensities were calculated from the plotted values in FIG. 12, and the values so calculated were plotted against the corresponding cycles.

FIG. 14 is a print-out of the graph prepared in step (g) based on the data processed in step (f) [step (h)]. Namely, it is a graph obtained by using a decrease of 0.5 in fluorescence intensity as a threshold, plotting along X-axis the number of cycles in which the threshold was reached, and also plotting along Y-axis the numbers of copies of the human genome DNA before the initiation of the respective reactions. The correlation coefficient (R2) of the line in this graph was calculated in step (i), and was then printed [step (j)]. The correlation coefficient was 0.9514. As is understood, it was hardly possible, with this correlation coefficient, to determine an accurate number of copies this correlation coefficient was

Example 22

This Example is directed to an experiment in which processing of data was performed by using the data analysis method of the present invention.

PCR was conducted in a similar manner as in Comparative

## Example 1.

The processing of the data was performed through similar steps as in Comparative Example 1 except that the following step (a) was added before the step (b) and the steps (b), (d) were modified as will be described below.

(a) The intensity of fluorescence in each cycle in a reaction system in which an amplified nucleic acid hybridized to a nucleic acid primer labeled with a fluorescent dye [namely, the intensity of fluorescence at the time of a nucleic acid extending reaction (72°C)] was corrected in a correction processing step such that the intensity of fluorescence was divided by the intensity of fluorescence in the reaction system measured at the time of dissociation of the hybrid complex of the amplified nucleic acid and the nucleic acid primer [namely, the intensity of fluorescence at the time of the nucleic acid denaturing reaction (95°C)], that is, the actually-measured intensities of fluorescence were corrected in accordance with the following formula (1):

$$f_n = f_{\text{hyb},n} / f_{\text{den},n} \quad (1)$$

where

$f_n$ : correction value for the intensity of fluorescence in each cycle,

$f_{\text{hyb},n}$ : the intensity of fluorescence at 72°C in each cycle, and

$f_{\text{den},n}$ : the intensity of fluorescence at 95°C in each

cycle.

It is FIG. 15 that was obtained by plotting the thus-obtained values against the corresponding cycles.

(b) A processing step that the values correction-processed  
5 by formula (1) in the respective cycles were introduced into the formula (3) to calculate the rates of changes (decreases or quenches, %) in fluorescence between the samples in the respective cycles, namely, a step for performing processing in accordance with the following formula (10):

10 
$$F_n = f_n / f_{25} \quad (10)$$

where

$F_n$ : processed value of each cycle,

$f_n$ : value of each cycle as obtained in accordance with formula (1), and

15  $f_{25}$ : value of the 25<sup>th</sup> cycle as obtained in accordance with formula (1).

Formula (10) is similar to formula 3 except for  $a=25$ .

(d) A step that the processed value of each cycle as obtained in step (b) was subjected to processing in accordance with  
20 formula (6) to obtain the logarithm of the rate of a change (decrease or quench, %) in fluorescence intensity, namely, a step for performing processing in accordance with the following formula (11):

$$\log \{(1-F_n) \times 100\} \quad (11)$$

25 where

000240 22195560

$F_n$ : value obtained in accordance with formula (10).

Formula (11) is similar to formula (6) except for  $b=10$  and  $A=100$ .

The above results are shown in FIGS. 16 and 17.

5            FIG. 16 is a print-out obtained by plotting the values, which have been processed in steps (a) and (b), against the corresponding cycles.

FIG. 17 is a print-out obtained by processing the values, which have been obtained in FIG. 16, in a similar manner as in step (d) and then plotting the thus processed values against the corresponding cycles.

Next, based on the graph of FIG. 17, processing was performed through steps (f), (g) and (h). Described specifically, as in Comparative Example 1, 0.1, 0.3, 0.5, 0.7, 0.9 and 1.2 were chosen as thresholds for log (rates of changes in fluorescence intensity, %). The numbers of cycles in which the logarithms reached the thresholds were plotted along X-axis, while the numbers of copies of the human genome DNA before the initiation of reactions were plotted along Y-axis, whereby working lines were drawn. The results are shown in FIG. 18. Correlation coefficients ( $R^2$ ) determined by conducting processing in steps (i) and (j) with respect to those working lines were 0.998, 0.999, 0.9993, 0.9985, 0.9989 and 0.9988, respectively. From those correlation coefficients, it was able to confirm that adoption of 0.5 as a threshold (correlation

coefficient: 0.9993) is desired. It is understood that, with a working line having this correlation coefficient, the number of copies before initiation of a reaction can be accurately determined with respect to a nucleic acid sample the number of  
5 copies of which is unknown.

#### Example 23

This Example is directed to an analysis of a melting curve of a nucleic acid and also to an analysis of a  $T_m$  value.

A software comprising the following steps was created:  
10 1) with respect to a nucleic acid amplified by the novel PCT method of the present invention, gradually heating the amplified nucleic acid from a low temperature until the nucleic acid is completely denatured (for example, from 50°C to 95°C), or gradually lowering it; 2) in step 1), measuring the intensity  
15 of fluorescence at short time intervals (for example, at intervals equivalent to temperature rises of from 0.2°C to 0.5°C); 3) displaying the measurement results of step 2) on a display as a function of time, namely, displaying a melting curve of the nucleic acid; 4) differentiating the melting curve  
20 obtained in step 3); 5) displaying, on a display, derivatives ( $-dF/dT$ , F: fluorescence intensity, T: time) obtained in step 4); and 6) determining a point of inflection from the derivatives obtained in step 5). Using "LightCycler™ System" (manufactured by Roche Diagnostics, Mannheim Germany) in which  
25 a computer-readable recording medium with the data analysis

000240 279550



software recorded therein had been installed, the novel real-time quantitative PCR reaction of the present invention was conducted to analyze the melting curve of the nucleic acid. In the present invention, the intensity of fluorescence  
5 increases with the temperature.

With respect to 1 copy and 10 copies of the same human genome DNA as in Example 22, PCR was conducted in a similar manner as in Example 20. FIG. 19 is a print-out of data obtained by processing data of the PCR in steps 1), 2), 3), 4) and 5).  
10 Concerning 75<sup>th</sup> amplification products of the 1 copy and 10 copies, data were processed in steps 1), 2 and 3) of this Example. The nucleic acid melting curves so obtained are shown in FIG. 20. Those curves were differentiated in step 4), and points of inflection ( $T_m$  values) were determined in step 5) and 6).  
15 The differentiated curves with the points of inflection are illustrated in FIG. 21. It was ascertained from FIG. 21 that the amplification products of the 1 copy and 10 copies were different products as their  $T_m$  values were different from each other.

## CLAIMS:

1. A method for determining a concentration of a target nucleic acid by using a nucleic acid probe labeled with a fluorescent dye, which comprises:

5 providing, as said probe, a nucleic acid probe capable of reducing fluorescence emission from said fluorescent dye when hybridized with said target nucleic acid;

hybridizing said probe to said target nucleic acid; and  
measuring a decrease in fluorescence emission from said  
10 fluorescent dye after said hybridization relative to fluorescence emission from said fluorescent dye before said hybridization.

2. A nucleic acid probe for determining a concentration of a target nucleic acid, said probe being labeled with a  
15 fluorescent dye, wherein:

said probe is labeled at an end portion thereof with said fluorescent dye, and

said probe has a base sequence designed such that, when said probe is hybridized with said target nucleic acid, at least  
20 one G (guanine) base exists in a base sequence of said target nucleic acid at a position 1 to 3 bases apart from an end base portion where said probe and said target nucleic acid are hybridized with each other;

whereby said fluorescent dye is reduced in fluorescence  
25 emission when said probe is hybridized with said target nucleic

000240 22195560

acid.

3. A nucleic acid probe according to claim 2, wherein said probe is labeled at a 3' end thereof with said fluorescent dye.

5 4. A nucleic acid probe according to claim 2, wherein said probe is labeled at a 5' end thereof with said fluorescent dye.

10 5. A nucleic acid probe for determining a concentration of a target nucleic acid, said probe being labeled with a fluorescent dye, wherein:

said probe is labeled at an end portion thereof with said fluorescent dye, and

15 said probe has a base sequence designed such that, when said probe is hybridized with said target nucleic acid, base pairs in a probe-nucleic acid hybrid complex form at least one G (guanine) and C (cytosine) pair at said end portion;

whereby said fluorescent dye is reduced in fluorescence emission when said probe is hybridized with said target nucleic acid.

20 6. A nucleic acid probe according to claim 5, wherein said probe has G or C as a 3' end base and is labeled at said 3' end thereof with said fluorescent dye.

25 7. A nucleic acid probe according to claim 5, wherein said probe has G or C as a 5' end base and is labeled at said 5' end thereof with said fluorescent dye.

000040" / 2299560

8. A nucleic acid probe according to claim 4 or 7, wherein a hydroxyl group on a 2' or 3' carbon of a ribose or a 3' carbon of a deoxyribose at a 3' end of said probe has been phosphorylated.

5 9. A nucleic acid probe according to any one of claims 1-8, wherein an oligoribonucleotide of said probe is a chemically-modified nucleic acid.

10 10. A nucleic acid probe according to any one of claims 2-8, wherein an oligonucleotide of said probe is a chemiric oligonucleotide comprising a ribonucleotide and a deoxyribonucleotide.

11. A nucleic acid probe according to claim 10, wherein said ribonucleotide is a 2'-O-methyloligoribonucleotide.

15 12. A method for determining a concentration of a target nucleic acid, which comprises hybridizing a nucleic acid probe according to any one of claims 2-8 to said target nucleic acid and measuring a decrease in fluorescence emission from said fluorescent dye after said hybridization relative to fluorescence emission from said fluorescent dye before said hybridization.

20 13. A method for determining a concentration of a target nucleic acid, which comprises:

hybridizing a nucleic acid probe according to any one of claims 9-11 to said target nucleic acid, and

25 measuring a decrease in fluorescence emission from said fluorescent dye after said hybridization relative to

000240 22195560

fluorescence emission from said fluorescent dye before said hybridization.

14. A method for analyzing or determining polymorphism or mutation of a target nucleic acid or gene, which comprises:

5            hybridizing a nucleic acid probe according to any one of  
claims 2-11 to said target nucleic acid or gene, and  
measuring a change in fluorescence.

15. A kit for analyzing or determining polymorphism or mutation of a target nucleic acid or gene, comprising a nucleic acid probe according to any one of claims 2-11.

16. A method for analyzing data obtained by an analysis or determination method according to claim 14, which comprises the following step:

correcting a fluorescence intensity of a reaction system,  
15 in which said target nucleic acid or gene has been hybridized  
with said nucleic acid probe labeled with said fluorescent dye,  
in accordance with a fluorescence intensity of said reaction  
system before said hybridization.

17. A system for analyzing or determining polymorphism  
20 or mutation of a target nucleic acid or gene, comprising means  
for practicing a data analysis or determination method  
according to claim 16.

18. A computer-readable, recording medium comprising a program recorded therein for making a computer perform a correction step as defined in claim 16.

19. A method according to claim 13, further comprising adding, before said hybridization, a helper probe to a reaction system in which said hybridization is conducted.

5 20. A method according to claim 13, wherein said nucleic acid probe and said target nucleic acid are hybridized after said target nucleic acid is subjected to heat treatment under conditions suited for sufficient degradation of a higher-order structure of said target nucleic acid.

10 21. A kit according to claim 15, further comprising a helper probe for being added to a hybridization reaction system.

22. A method according to claim 12, 13, 19 or 20, wherein said target nucleic acid is RNA.

23. A device for determining concentrations of nucleic acids, comprising:

15 a solid support, and

a nucleic acid probe according to any one of claims 2-11 or a different nucleic acid probe bound on a surface of said solid support, said different nucleic acid probe having a structure designed such that said probe comprises two  
20 fluorescent dyes of different kinds in a molecule and that, owing to interaction between said two fluorescent dyes, said probe quenches or emits fluorescence when said probe is not hybridized with said target nucleic acid but emits fluorescence or quenches when said probe is hybridized with said target  
25 nucleic acid;

whereby said device can determine said concentration of said target nucleic acid by hybridizing said target nucleic acid to said probe or said different probe.

24. A device according to claim 23, wherein said probes  
5 or said different probes are arranged and bound in an array  
pattern on said surface of said solid support.

25. A device according to claim 23 or 24, wherein said probes or different probes bound on said surface of said solid support are each independently provided with at least one temperature sensor and at least one heater arranged on an opposite surface of said solid support such that an area of said solid support, where said probe or different probe is bound, can be controlled to meet optimal temperature conditions.

26. A device according to any one of claims 23 to 25,  
15 wherein said probes or different probes are bound at end  
portions, where said probes or different probes are labeled with  
no fluorescent dye, on said surface of said solid support.

27. A method for determining a concentration of a target nucleic acid, which comprises determining said concentration of said target nucleic acid by using a device according to any one of claims 23-26.

28. A method according to any one of claims 1, 12, 13, 19-22 and 27, wherein said target nucleic acid is a nucleic acid derived from a microorganism or animal and obtained by pure  
25 purification.

5

10

15

20

25

measuring an intensity of fluorescence of a reaction system in which said probe and said target nucleic acid or



amplified nucleic acid have not hybridized with each other and also an intensity of fluorescence of said reaction system in which said probe and said target nucleic acid or amplified nucleic acid have hybridized with each other; and then

5           calculating a decrease of said former intensity of fluorescence from said latter intensity of fluorescence.

32. A method according to claim 30 or 31, wherein said PCR is real-time quantitative PCR.

33. A method for analyzing data obtained by a  
10           determination method according to any one of claims 1, 12, 13, 19-22 and 27-32, further comprising correcting an intensity value of fluorescence of a reaction system, said intensity value being available after said target nucleic acid has hybridized to said nucleic acid probe labeled with said fluorescent dye,  
15           in accordance with an intensity value of fluorescence of said reaction system available after a probe-nucleic acid hybrid complex so formed has dissociated.

34. A method for analyzing data obtained by a real-time quantitative PCR method according to claim 32, further  
20           comprising, as a correction processing step, correcting an intensity value of fluorescence of a reaction system, said intensity being available in each cycle after said amplified nucleic acid has conjugated to said fluorescent dye or after said amplified nucleic acid has hybridized to said nucleic acid  
25           probe labeled with said fluorescent dye, in accordance with an

000240 229560

intensity value of fluorescence of said reaction system available after a nucleic acid-fluorescent dye conjugate or probe-nucleic acid hybrid complex so formed has dissociated in said cycle.

- 5           35. A method according to claim 34, wherein said correction-processing step is performed in accordance with the following formula (1) or formula (2):

$$f_n = f_{hyb,n} / f_{den,n} \quad (1)$$

$$f_n = f_{den,n} / f_{hyb,n} \quad (2)$$

10       where

$f_n$ :       correction-processed value in an  $n^{th}$  cycle as calculated in accordance with the formula (1) or formula (2),

15        $f_{hyb,n}$ : intensity value of fluorescence of the reaction system available after said amplified nucleic acid has conjugated to said fluorescent dye or said amplified nucleic acid has hybridized to said nucleic acid probe labeled with said fluorescent dye in said  $n^{th}$  cycle, and

20        $f_{den,n}$ : intensity value of fluorescence of the reaction system available after said nucleic acid-fluorescent dye conjugate has dissociated in said  $n^{th}$  cycle or said probe-nucleic acid hybrid complex has dissociated in said  $n^{th}$  cycle.

- 25           36. A method according to claim 35, which comprises:

introducing correction-processed values, which have been calculated in accordance with the formula (1) or formula (2) in individual cycles, into the following formula (3) or (4) to calculate rates or percentages of changes in fluorescence between samples in said individual cycles:

$$F_n = f_n / f_a \quad (3)$$

$$F_n = f_a / f_n \quad (4)$$

where

$F_n$ : rate or percentage of a change in fluorescence in an  $n^{\text{th}}$  cycle as calculated in accordance with the formula (3) or formula (4),

$f_n$ : correction-processed value calculated in said  $n^{\text{th}}$  cycle as calculated in accordance with the formula (1) or formula (2), and

$f_a$ : correction-processed value calculated in a given cycle before a change in  $f_n$  is observed as calculated in accordance with the formula (1) or formula (2); and comparing said rates or percentages of changes in fluorescence.

37. A method according to claim 36, which comprises the following processing steps:

1) performing processing in accordance with the following formula (5), (6) or (7) by using data of rates or percentages of changes in fluorescence as calculated in accordance with said formula (3) or (4):

$$\log_b(F_n), \ln(F_n) \quad (5)$$

$$\log_b\{(1-F_n) \times A\}, \ln\{(1-F_n) \times A\} \quad (6)$$

$$\log_b\{(F_n-1) \times A\}, \ln\{(F_n-1) \times A\} \quad (7)$$

where

5        A,b: desired numerical values, and

$F_n$ : rate or percentage of a change in fluorescence in an  
           $n^{\text{th}}$  cycle as calculated in accordance with the formula  
          (3) or formula (4),

10        2) determining a cycle in which said processed value of  
          said processing step 1) has reached a constant value,

      3) calculating a relational expression between cycle of  
a nucleic acid sample of a known concentration and the number  
of copies of said target nucleic acid at the time of initiation  
of a reaction, and

15        4) determining the number of copies of said target nucleic  
acid in an unknown sample upon initiation of PCR.

38. A method for analyzing a melting curve of a target  
nucleic acid, which comprises:

20        performing PCR on said target nucleic acid by using a  
nucleic acid probe according to any one of claims 2-11; and  
analyzing said melting curve of said target nucleic acid  
to determine a  $T_m$  value of each amplified nucleic acid.

39. A method for analyzing a melting curve of a target  
nucleic acid, which comprises:

25        performing PCR on said target nucleic acid by using a

000240 229550

nucleic acid probe according to claim 4 or 7 as a primer; and  
analyzing said melting curve of said target nucleic acid  
to determine a  $T_m$  value of each amplified nucleic acid.

40. A data analyzing method for a real-time quantitative  
5 PCR method according to claims 34-37, which comprises the  
following steps:

gradually heating a PCR-amplified nucleic acid from a low  
temperature until complete denaturation of said nucleic acid;

10 measuring an intensity of fluorescence at predetermined  
time intervals during said heating step;

displaying results of said measurement as a function of  
time on a display such that a melting curve of said nucleic acid  
is drawn on said display;

15 differentiating said melting curve to obtain  
differentiated values ( $-dF/dT$ ,  $F$ : intensity of fluorescence,  
 $T$ : time);

displaying said differentiated values as derivatives on  
said display; and

determining a point of inflection from said derivatives.

20 41. A determining and/or analyzing system for real-time  
quantitative PCR, comprising:

means for performing a data analysis step by a data  
analysis method according to claim 34;

25 means for performing a data analysis step by a data  
analysis method according to claim 35;

means for performing a data analysis step by a data analysis method according to claim 36;

means for performing a data analysis step by a data analysis method according to claim 37; and

5 means for performing a data analysis step by a data analysis method according to claim 40.

42. A computer-readable recording medium comprising a program recorded therein for making a computer perform the following steps:

10 analysis of data by a data analysis method according to claim 34;

analysis of data by a data analysis method according to claim 35;

15 analysis of data by a data analysis method according to claim 36;

analysis of data by a data analysis method according to claim 37; and

analysis of data by a data analysis method according to claim 40.

20 43. A method for quantitating a nucleic acid, which comprises using a data analysis method according to any one of claims 34-37 and 40 for real-time quantitative PCR.

44. A method for quantitating a nucleic acid, which comprises using a system according to claim 41.

25 45. A method for quantitating a nucleic acid, which

0000240 0425560

122

comprises using a computer-readable recording medium according to claim 42.

000240" 2255550

## ABSTRACT

A method is provided for determining a concentration of a target nucleic acid by using a nucleic acid probe labeled with a fluorescent dye. The method comprises:

5 providing, as the probe, a nucleic acid probe capable of reducing fluorescence emission from the fluorescent dye when hybridized with the target nucleic acid;

10 hybridizing the probe to the target nucleic acid; and measuring a decrease in fluorescence emission from the fluorescent dye after the hybridization relative to fluorescence emission from the fluorescent dye before the hybridization.

0000240" 234560



FIG.1

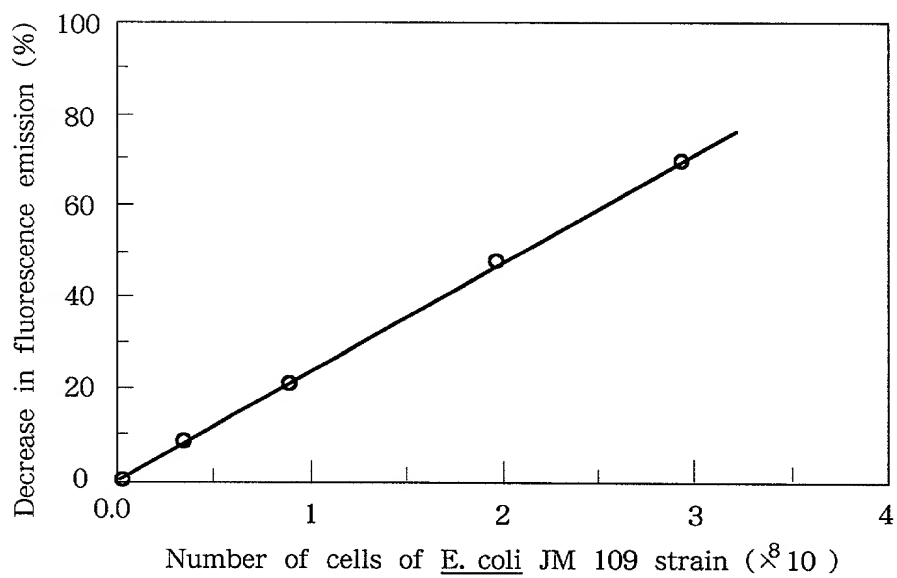


FIG.2


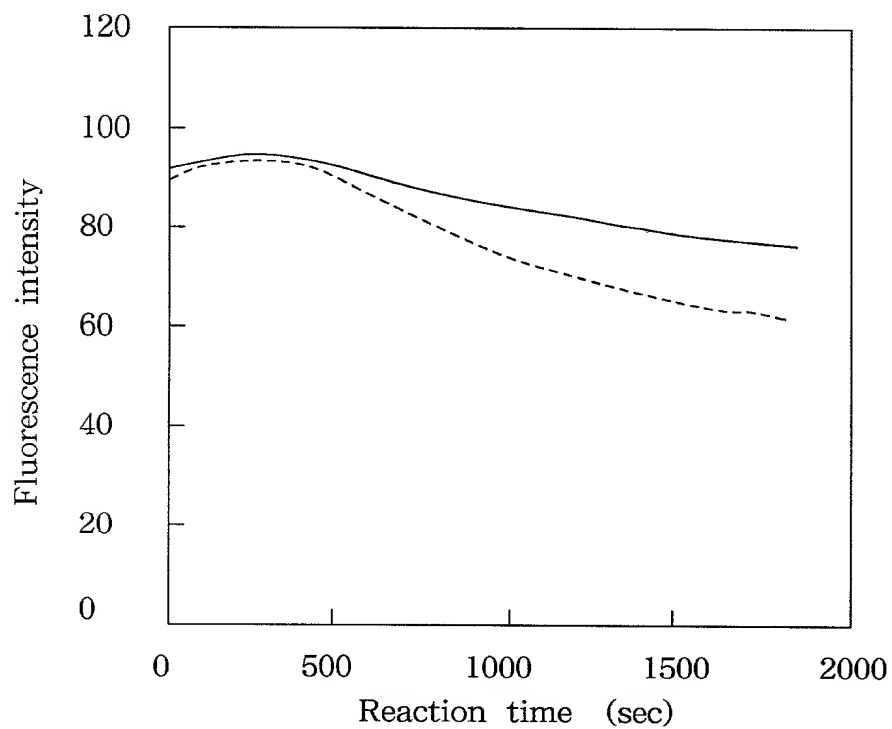


FIG.3

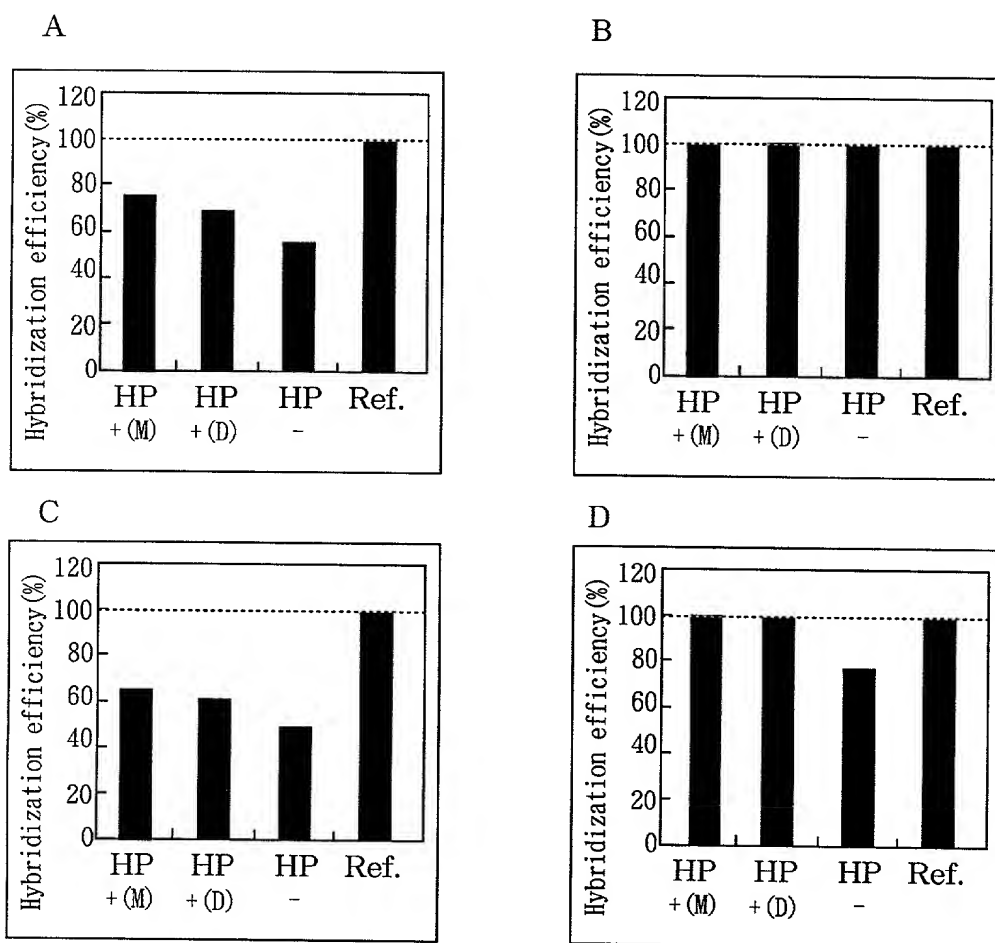

A : 35 - nucleotides - chained deoxyriboligonucleic acid probe

B : 35 - nucleotides - chained 2 - O - Me probe

C : 17 - nucleotides - chained deoxyriboligonucleic acid probe

D : 17 - nucleotides - chained 2 - O - Me probe

HP : Helper probe

HP + (M) : Helper probe + 2 - O - Me probe

HP + (D) : Helper probe + deoxyribooligonucleotide probe

Ref. : Reference

FIG.4

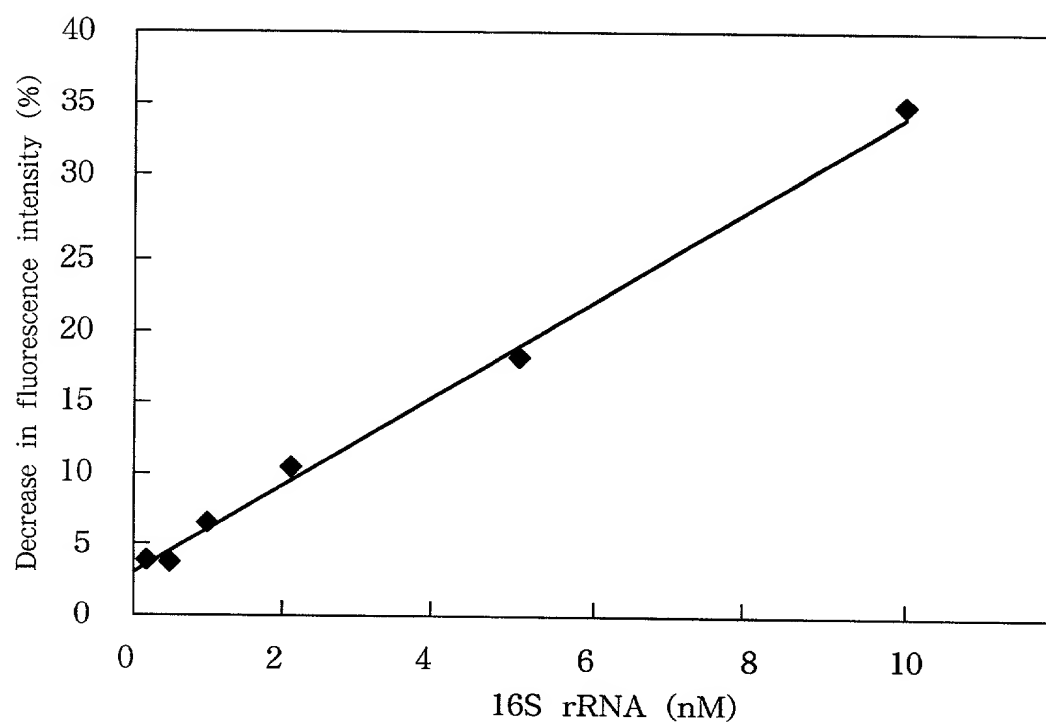


FIG.5

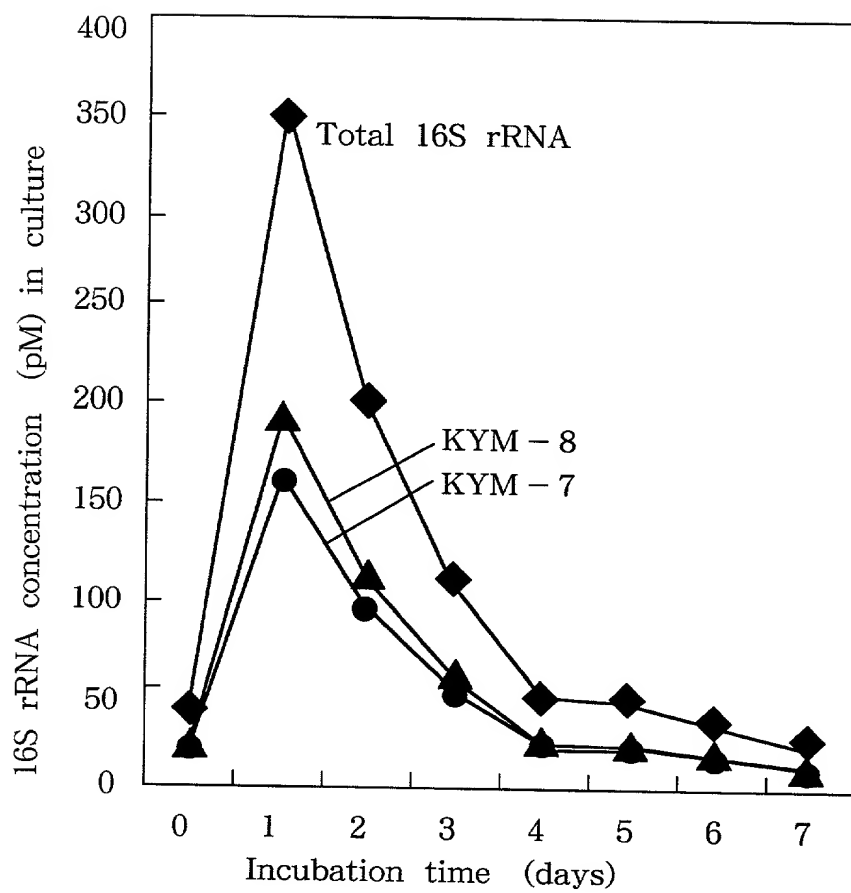


FIG.6

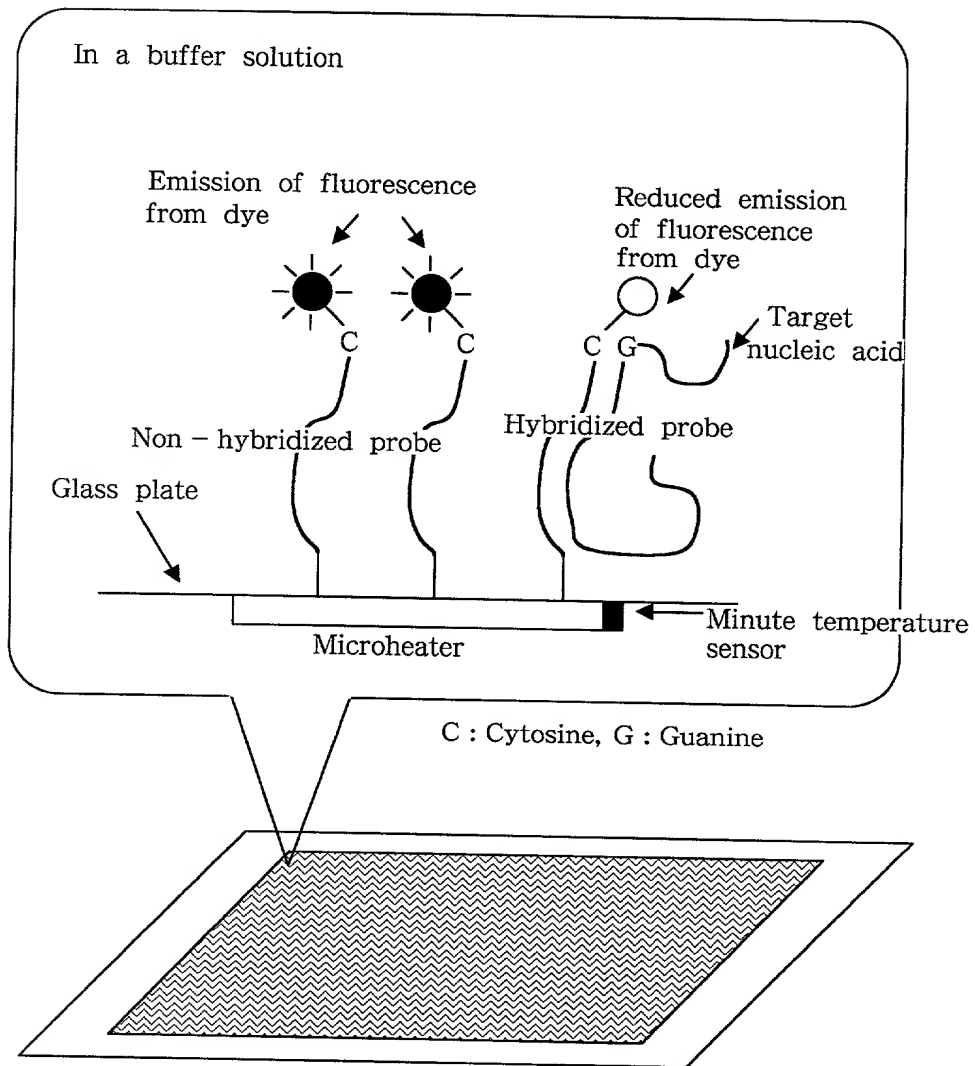


FIG.7

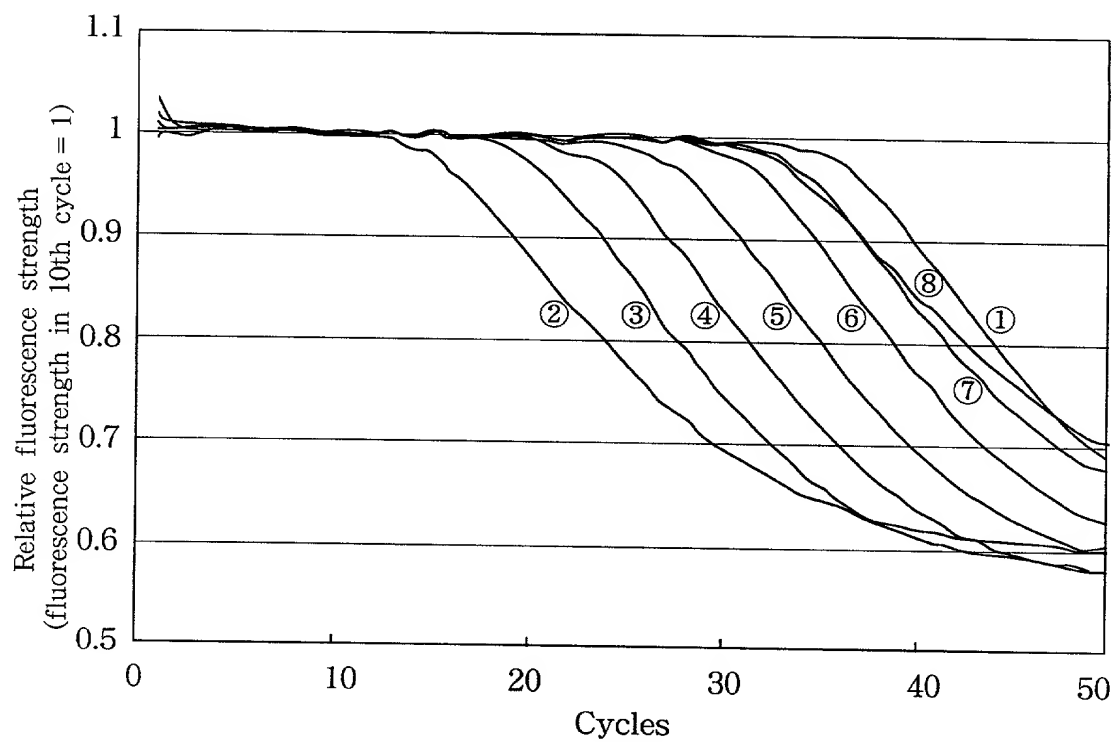


FIG.8

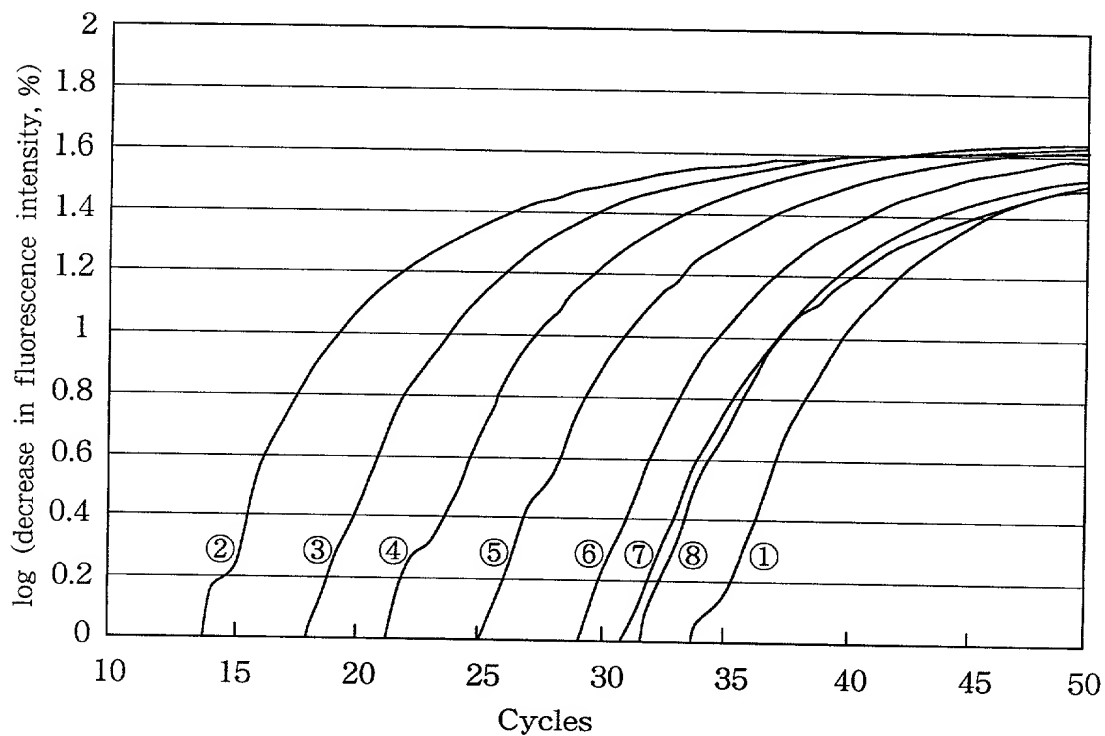


FIG.9

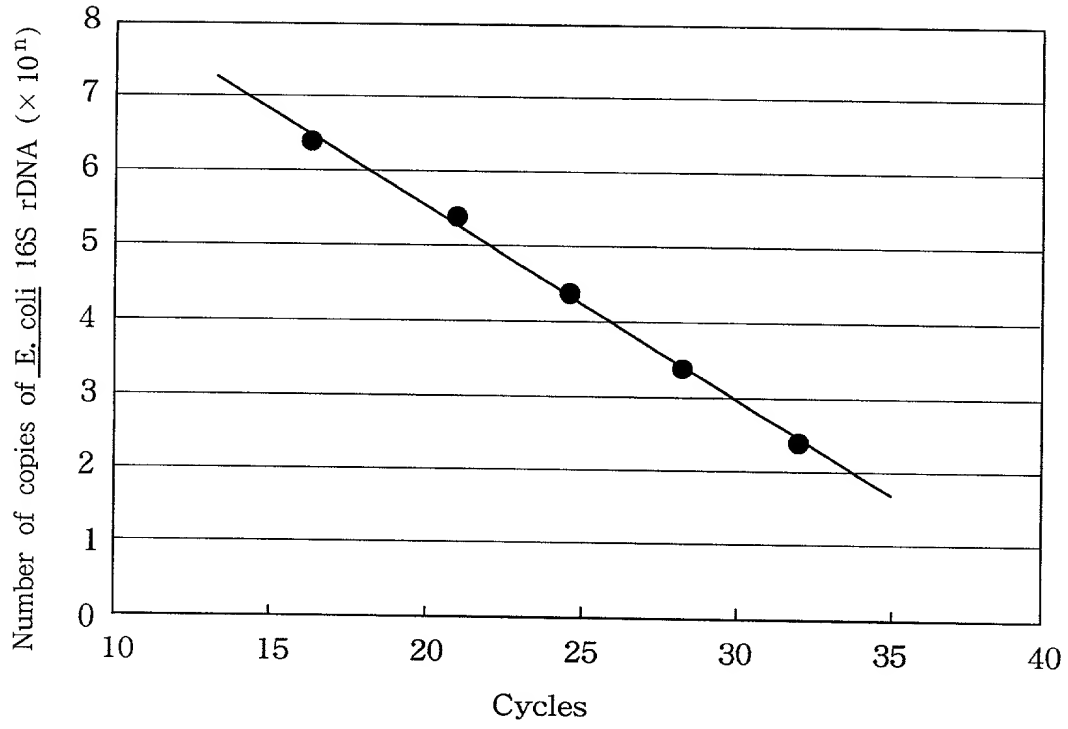


FIG.10

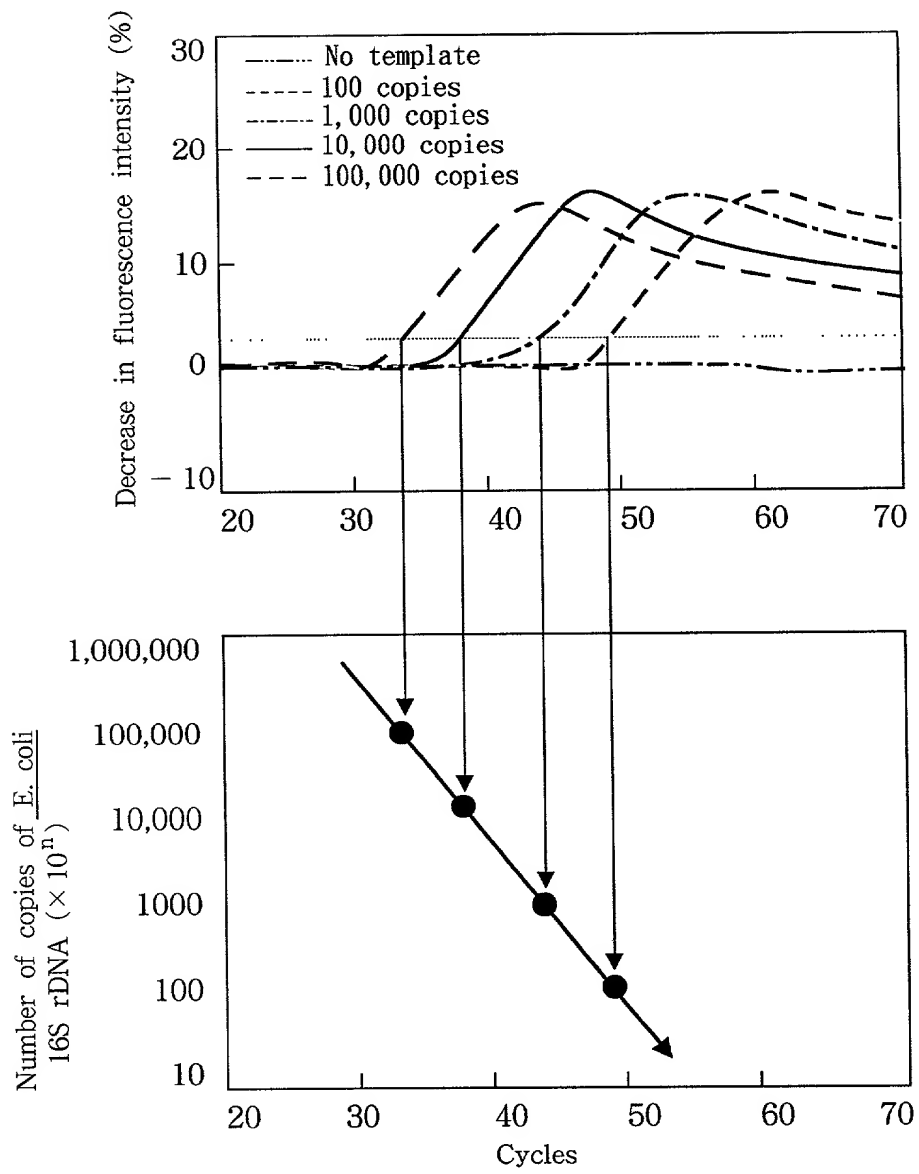




FIG.11

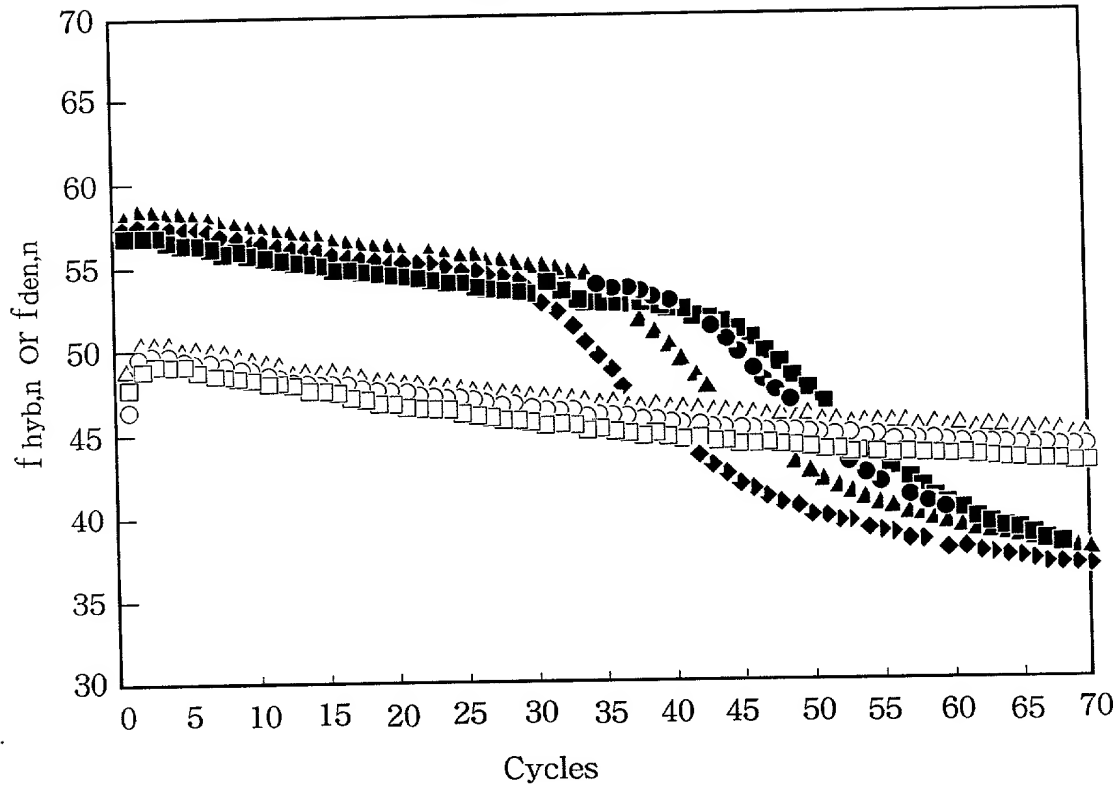


FIG.12

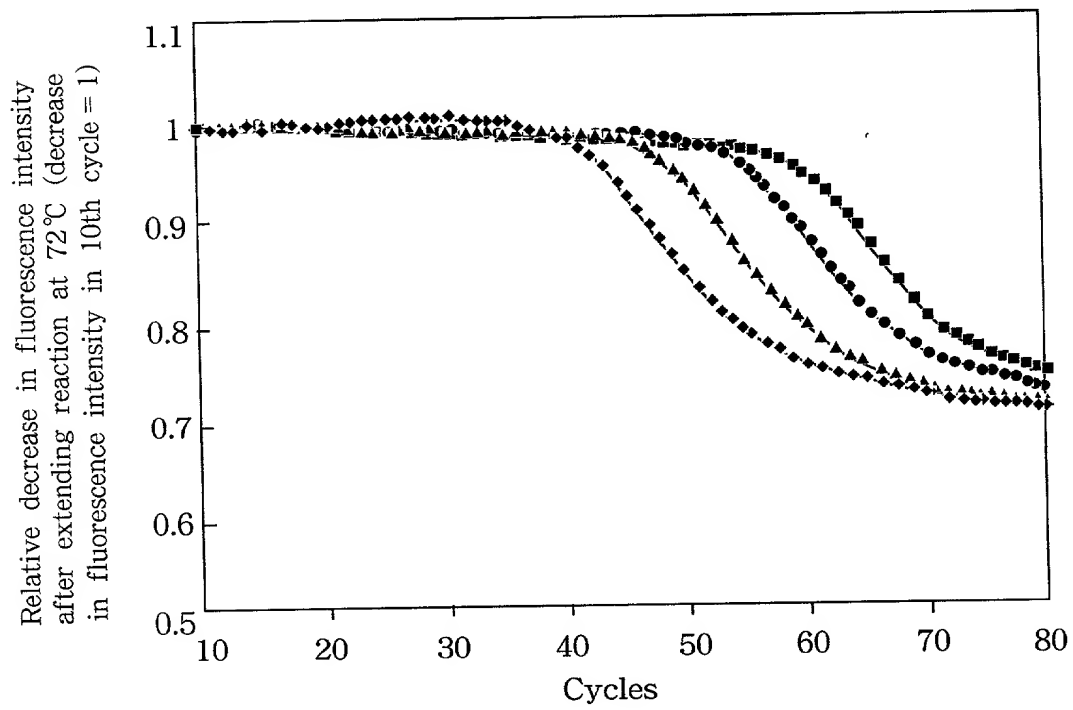


FIG.13

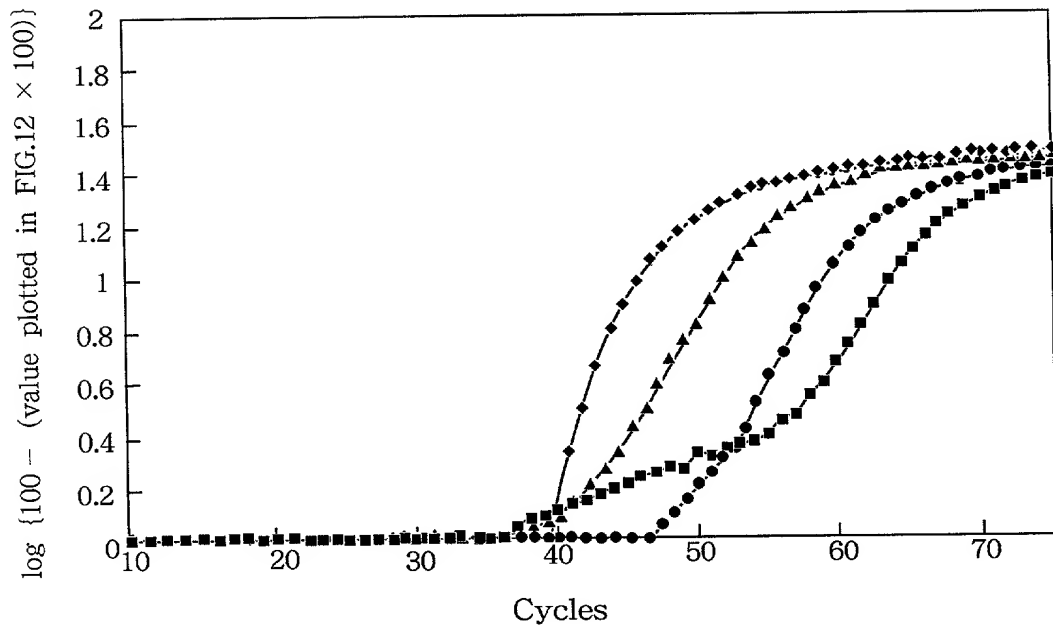


FIG.14

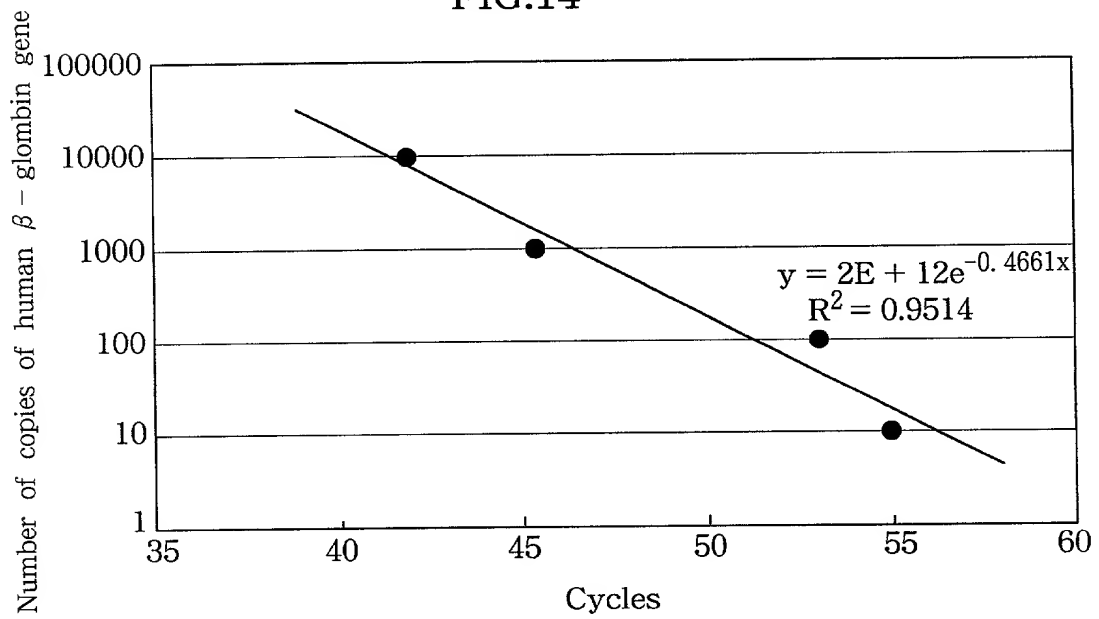


FIG.15

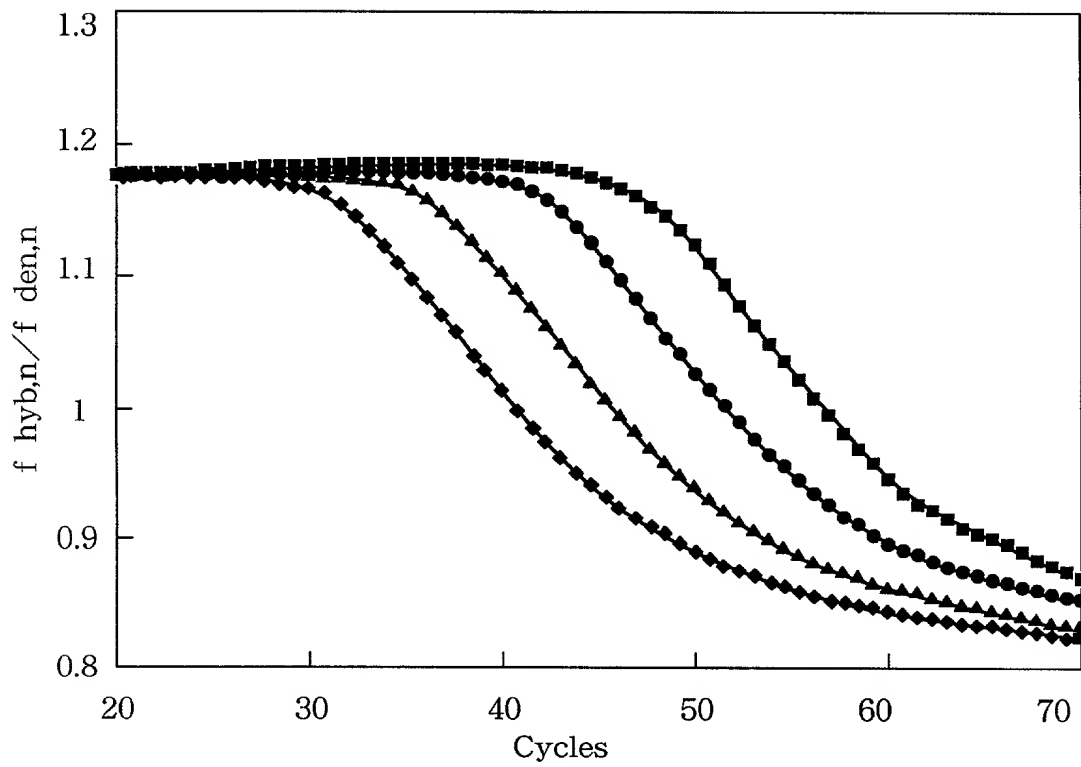


FIG.16

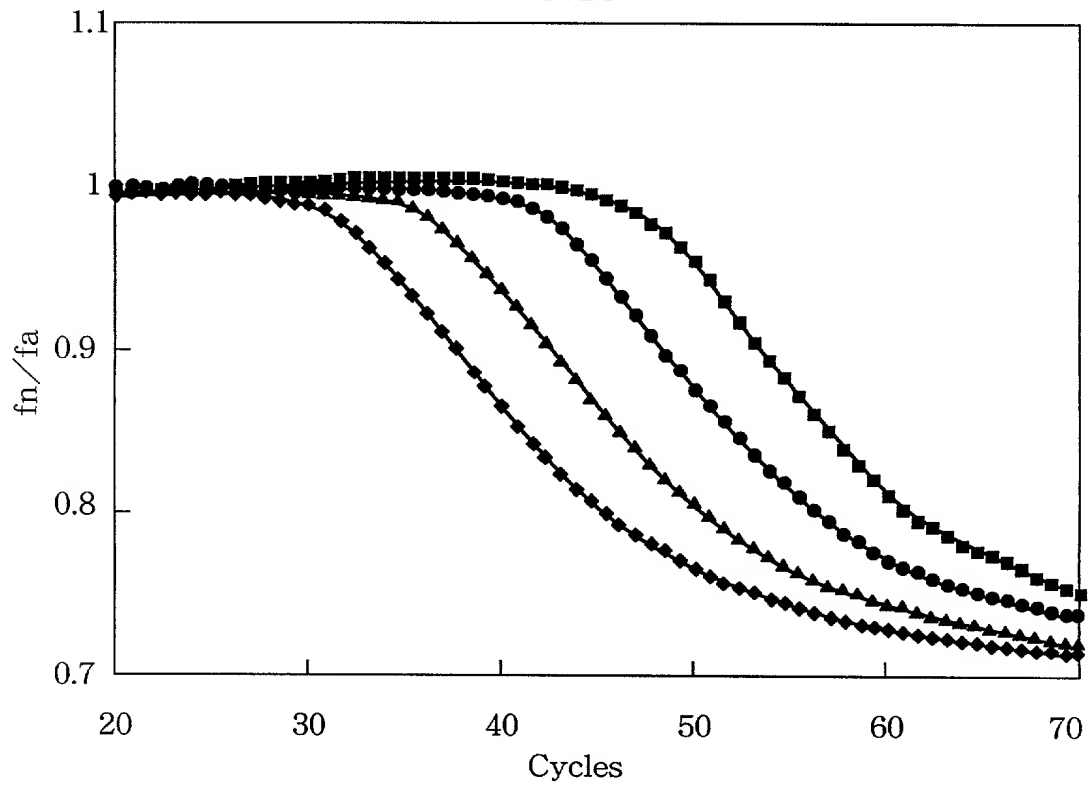


FIG.17

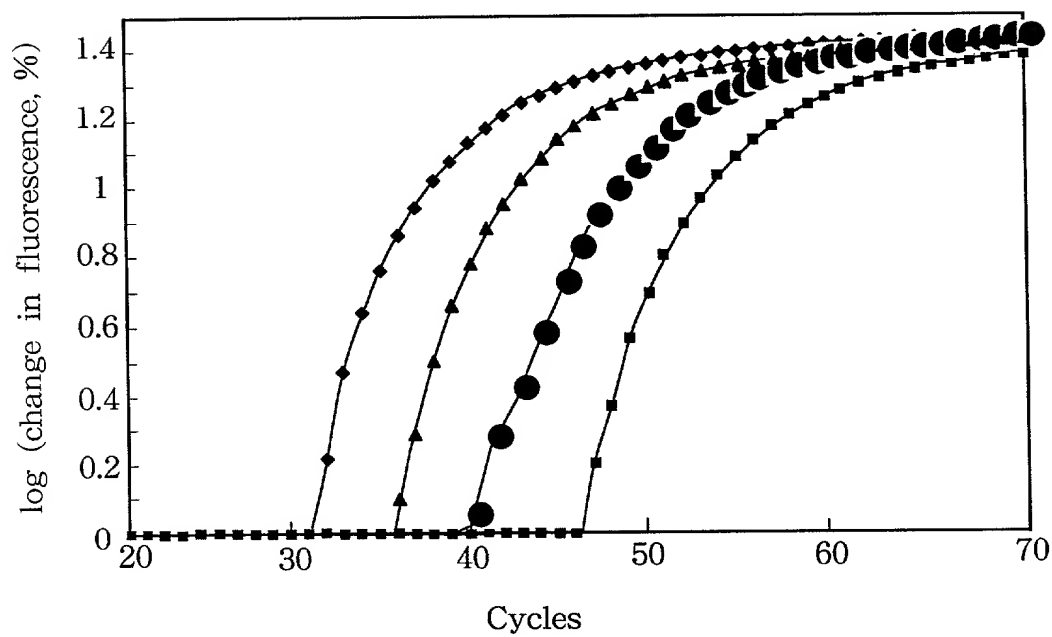


FIG.18

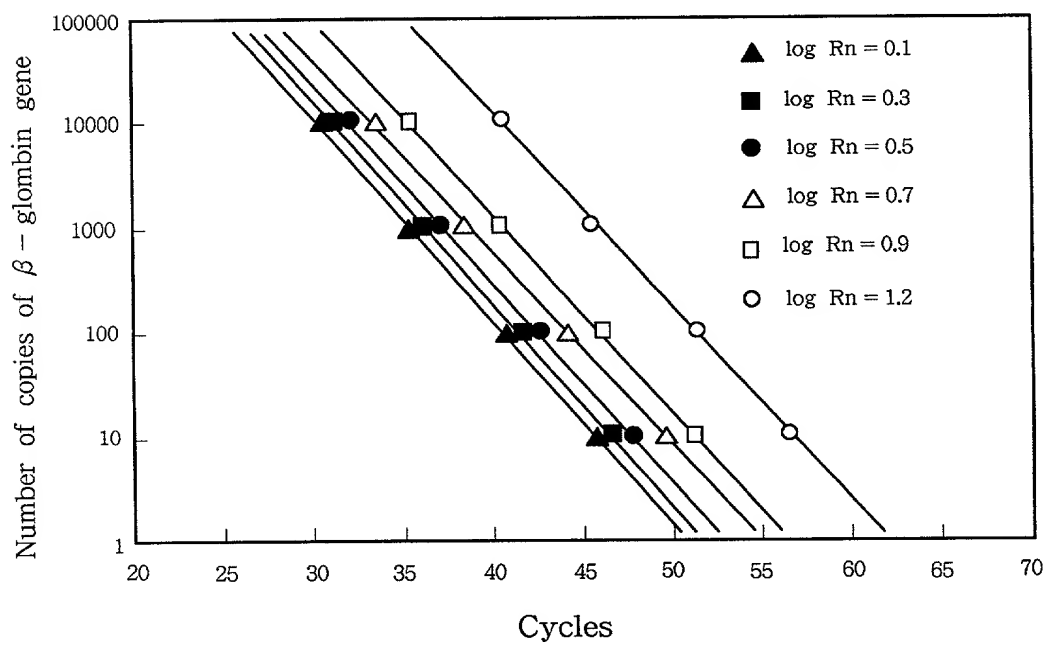


FIG.19

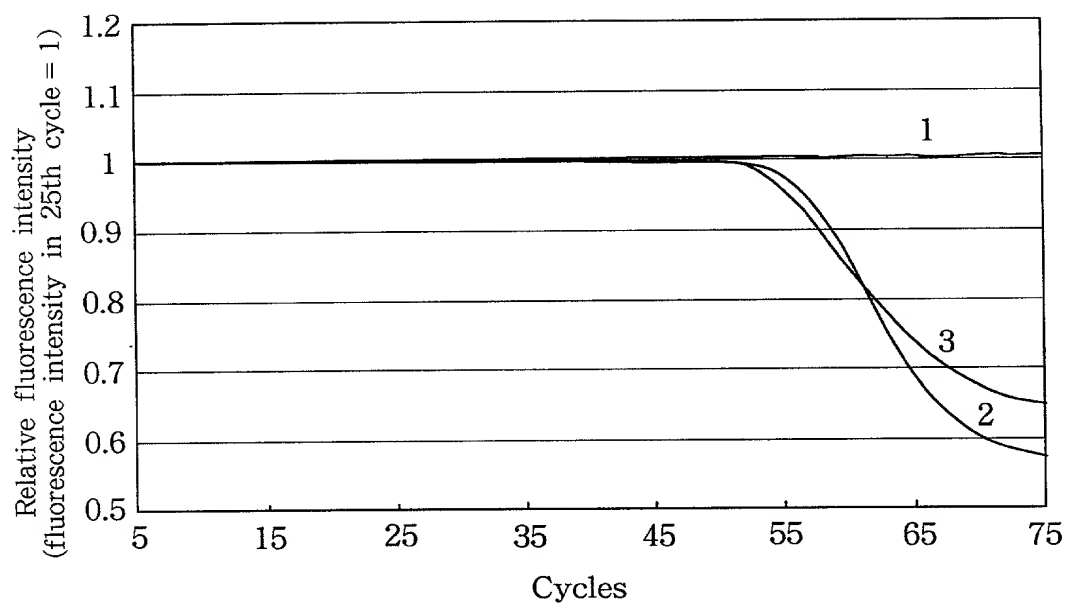


FIG.20


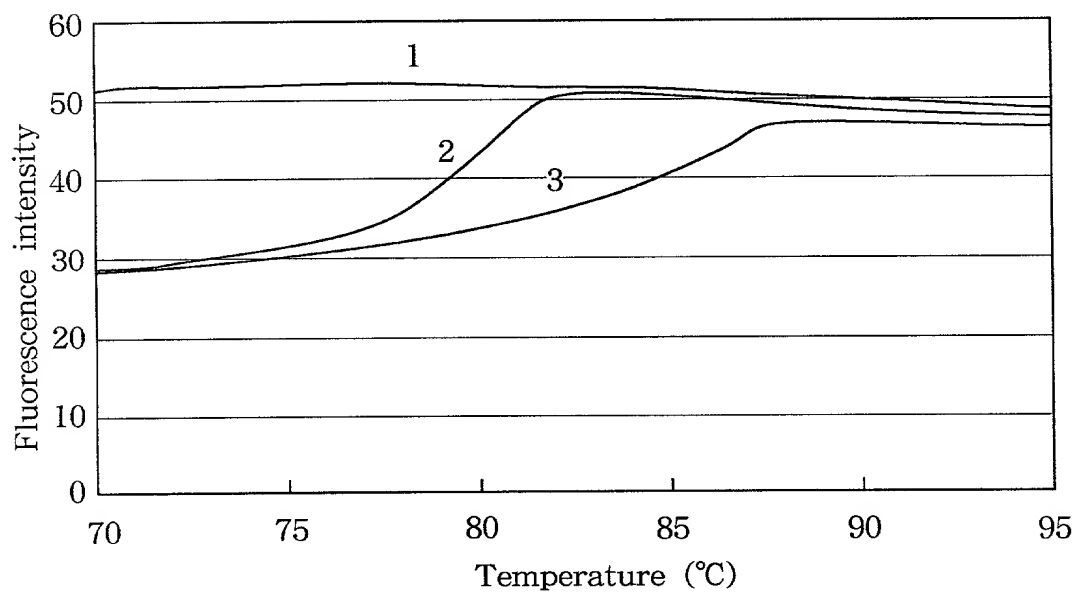


FIG.21

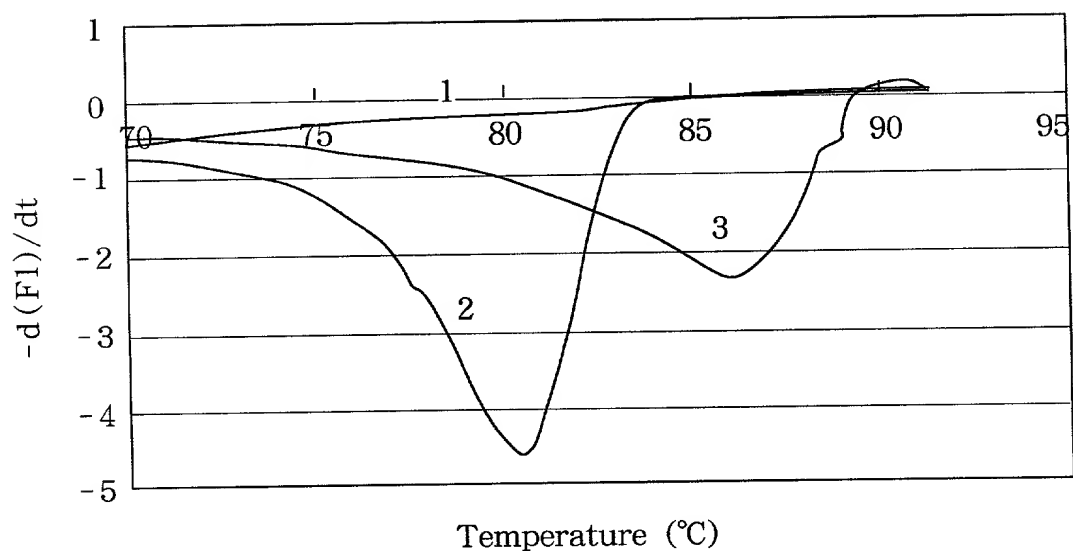

**IN THE UNITED STATES PATENT AND TRADEMARK OFFICE**

IN RE APPLICATION OF: RYUICHIRO KURANE ET AL

FILING DATE: Herewith

FOR: METHOD FOR DETERMINING A CONCENTRATION OF TARGET NUCLEIC ACID MOLECULES,  
NUCLEIC ACID PROBES FOR THE METHOD, AND METHOD FOR ANALYZING DATA OBTAINED  
BY THE METHOD

**LIST OF INVENTORS' NAMES AND ADDRESSES**

ASSISTANT COMMISSIONER FOR PATENTS  
WASHINGTON, D.C. 20231

SIR:

Listed below are the names and addresses of the inventors for the above-identified patent application.

Ryuichiro KURANE	C/O National Institute of Bioscience and Human- Technology 1-3, Higashi 1-chome Tukuba-shi Ibaraki 305-8566 Japan
Takahiro KANAGAWA	C/O National Institute of Bioscience and Human- Technology 1-3, Higashi 1-chome Tukuba-shi Ibaraki 305-8566 Japan
Yoichi KAMAGATA	C/O National Institute of Bioscience and Human- Technology 1-3, Higashi 1-chome Tukuba-shi Ibaraki 305-8566 Japan
Shinya KURATA	C/O Kankyo Engineering Co., Ltd. 1-9-8, Higashi-kanda, Chiyoda-ku Tokyo 101-0031 Japan
Kazutaka YAMADA	C/O Kankyo Engineering Co., Ltd. 1-9-8, Higashi-kanda, Chiyoda-ku Tokyo 101-0031 Japan
Toyokazu YOKOMAKU	C/O Kankyo Engineering Co., Ltd. 1-9-8, Higashi-kanda, Chiyoda-ku Tokyo 101-0031 Japan
Osamu KOYAMA	C/O Kankyo Engineering Co., Ltd. 1-9-8, Higashi-kanda, Chiyoda-ku Tokyo 101-0031 Japan

C/O Kankyo Engineering Co., Ltd.  
1-9-8, Higashi-kanda, Chiyoda-ku  
Tokyo 101-0031 Japan

Respectfully Submitted,

David J. H.

Fourth Floor  
1755 Jefferson Davis Highway  
Arlington, Virginia 22202  
Tel. (703) 413-3000  
Fax. (703) 413-2220  
(OSMMN 11/98)

Daniel J. Pereira, Ph.D.  
Registration No. 45,518

[illegible]